

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
11 March 2004 (11.03.2004)


PCT

(10) International Publication Number
WO 2004/019816 A2

- (51) International Patent Classification⁷: **A61F 2/00**
- (21) International Application Number: **PCT/US2003/027278**
- (22) International Filing Date: **29 August 2003 (29.08.2003)**
- (25) Filing Language: **English**
- (26) Publication Language: **English**
- (30) Priority Data:
- | | | |
|------------|-------------------------------|----|
| 60/406,841 | 29 August 2002 (29.08.2002) | US |
| 60/444,005 | 31 January 2003 (31.01.2003) | US |
| 60/447,383 | 14 February 2003 (14.02.2003) | US |
| 60/462,435 | 12 April 2003 (12.04.2003) | US |
- (71) Applicant (for all designated States except US): **MD3 TECHNOLOGIES LLC [US/US]; Suite 3000, Five Concourse Parkway, Atlanta, GA 30328 (US).**
- (72) Inventors; and
- (75) Inventors/Applicants (for US only): **CARTLEDGE, Richard, G. [US/US]; 1554 Yellow Heart Way, Hollywood, FL 30328 (US). LEE, Leonard, Y. [US/US]; 435 East 70th Street #12-L, New York, NY 10021 (US).**
- (74) Agents: **ROBERTS, Larry, A. et al.; 1100 Peachtree Street, Suite 2800, Atlanta, GA 30309 (US).**
- (81) Designated States (national): **AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.**
- (84) Designated States (regional): **ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).**
- Published:**
— without international search report and to be republished upon receipt of that report

[Continued on next page]

(54) Title: **IMPLANTABLE DEVICES FOR CONTROLLING THE INTERNAL CIRCUMFERENCE OF AN ANATOMIC ORIFICE OR LUMEN**

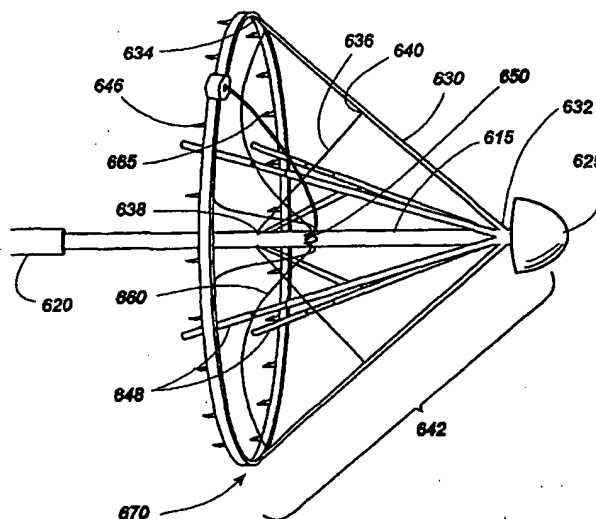

(57) Abstract: An implantable device for controlling the circumference of internal anatomic passages corrects physiologic dysfunctions resulting from a structural lumen which is either too large or too small. Implants are disclosed which employ various means for adjusting and maintaining the size of an orifice to which they are attached. Systems permit the implants to be implanted using minimally invasive procedures and permit final adjustments to the circumference of the implants after the resumption of normal flow of anatomic fluids in situ. Methods are disclosed for using the implants to treat heart valve abnormalities, gastroesophageal abnormalities, anal incontinence, and the like.

WO 2004/019816 A2



For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

IMPLANTABLE DEVICES FOR CONTROLLING THE INTERNAL CIRCUMFERENCE OF AN ANATOMIC ORIFICE OR LUMEN

5

TECHNICAL FIELD

The present invention relates generally to implantable devices and procedures and relates more specifically to implantable devices and procedures for controlling the internal circumference of an anatomic orifice or lumen.

10

BACKGROUND OF THE INVENTION

Many anatomic structures in the mammalian body are hollow passages in which walls of tissue define a central lumen, which serves as a conduit for blood, other physiologic fluids, nutrient matter, or waste matter passing within the structure. In many physiologic settings, dysfunction may result from a structural lumen which is either too large or too small. In most such cases, dysfunction can be relieved by interventional changes in the luminal size.

Thus in surgery, there is often a need to reduce the internal circumference of an orifice or other open anatomic structure to narrow the size of the orifice or opening to achieve a desired physiologic effect. Often, such surgical procedures require interruption in the normal physiologic flow of blood, other physiologic fluids, or other structural contents through the orifice or structure. The exact amount of the narrowing required for the desired effect often cannot be fully appreciated until physiologic flow through the orifice or structure is resumed. It would be advantageous, therefore, to have an adjustable means of achieving this narrowing effect, such that the degree of narrowing could be changed after its implantation, but after the resumption of normal flow *in situ*.

One example of a dysfunction within an anatomic lumen is in the area of cardiac surgery, and specifically valvular repair. Approximately one million open heart surgical procedures are now performed annually in the United States, and twenty percent of these operations are related to cardiac valves.

The field of cardiac surgery was previously transformed by the introduction of the pump oxygenator, which allowed open heart surgery to be performed. Valvular heart surgery was made possible by the further introduction of the mechanical ball-valve prosthesis, and many modifications and different forms of prosthetic heart valves have since been developed. However, the ideal prosthetic valve has yet to be designed, which attests to the elegant form and

function of the native heart valve. As a result of the difficulties in engineering a perfect prosthetic heart valve, there has been growing interest in repairing a patient's native valve. These efforts have documented equal long-term durability to the use of mechanical prostheses, with added benefits of better ventricular performance due to preservation of the subvalvular mechanisms and obviation of the need for chronic anticoagulation. Mitral valve repair has become one of the most rapidly growing areas in adult cardiac surgery today.

Mitral valve disease can be subdivided into intrinsic valve disturbances and pathology extrinsic to the mitral valve ultimately affecting valvular function. Although these subdivisions exist, many of the repair techniques and overall operative approaches are similar in the various pathologies that exist.

Historically, most valvular pathology was secondary to rheumatic heart disease, a result of a streptococcal infection, most commonly affecting the mitral valve, followed by the aortic valve, and least often the pulmonic valve. The results of the infectious process are mitral stenosis and aortic stenosis, followed by mitral insufficiency and aortic insufficiency. With the advent of better antibiotic therapies, the incidence of rheumatic heart disease is on the decline, and accounts for a smaller percentage of valvular heart conditions in the developed world of the present day. Commissurotomy of rheumatic mitral stenosis was an early example of commonly practiced mitral valve repair outside of the realm of congenital heart defects. However, the repairs of rheumatic insufficient valves have not met with good results due to the underlying valve pathology and the progression of disease.

Most mitral valve disease other than rheumatic results in valvular insufficiency that is generally amenable to repair. Chordae rupture is a common cause of mitral insufficiency, resulting in a focal area of regurgitation. Classically, one of the first successful and accepted surgical repairs was for ruptured chordae of the posterior mitral leaflet. The technical feasibility of this repair, its reproducible good results, and its long-term durability led the pioneer surgeons in the field of mitral valve repair to attempt repairs of other valve pathologies.

Mitral valve prolapse is a fairly common condition that leads over time to valvular insufficiency. In this disease, the plane of coaptation of the anterior and posterior leaflets is "atrialized" relative to a normal valve. This problem may readily be repaired by restoring the plane of coaptation into the ventricle.

The papillary muscles within the left ventricle support the mitral valve and aid in its function. Papillary muscle dysfunction, whether due to infarction or ischemia from coronary artery disease, often leads to mitral insufficiency (commonly referred to as ischemic mitral insufficiency). Within the scope of

mitral valve disease, this is the most rapidly growing area for valve repair. Historically, only patients with severe mitral insufficiency were repaired or replaced, but there is increasing support in the surgical literature to support valve repair in patients with moderate insufficiency that is attributable to
5 ischemic mitral insufficiency. Early aggressive valve repair in this patient population has been shown to increase survival and improve long-term ventricular function.

In addition, in patients with dilated cardiomyopathy the etiology of mitral
10 insufficiency is the lack of coaptation of the valve leaflets from a dilated ventricle. The resultant regurgitation is due to the lack of coaptation of the leaflets. There is a growing trend to repair these valves, thereby repairing the insufficiency and restoring ventricular geometry, thus improving overall ventricular function.

The two essential features of mitral valve repair are to fix primary valvular
15 pathology (if present) and to support the annulus or reduce the annular dimension using a prosthesis that is commonly in the form of a ring or band. The problem encountered in mitral valve repair is the surgeon's inability to fully assess the effectiveness of the repair until the heart has been fully closed, and the patient is weaned off cardiopulmonary bypass. Once this has been achieved,
20 valvular function can be assessed in the operating room using transesophageal echocardiography (TEE). If significant residual valvular insufficiency is then documented, the surgeon must re-arrest the heart, re-open the heart, and then re-repair or replace the valve. This increases overall operative, anesthesia, and bypass times, and therefore increases the overall operative risks.

If the prosthesis used to reduce the annulus is larger than the ideal size,
25 mitral insufficiency may persist. If the prosthesis is too small, mitral stenosis may result. The need exists, therefore, for an adjustable prosthesis that would allow a surgeon to adjust the annular dimension *in situ* in a beating heart under TEE guidance or other diagnostic modalities to achieve optimal valvular
30 sufficiency and function.

Cardiac surgery is but one example of a setting in which adjustment of the annular dimension of an anatomic orifice *in situ* would be desirable. Another
example is in the field of gastrointestinal surgery, where the Nissen fundoplication procedure has long been used to narrow the gastro-esophageal
35 junction for relief of gastric reflux into the esophagus. In this setting, a surgeon is conventionally faced with the tension between creating sufficient narrowing to achieve reflux control, but avoiding excessive narrowing that may interfere with the passage of nutrient contents from the esophagus into the stomach. Again, it would be desirable to have a method and apparatus by which the extent to which

the gastro-esophageal junction is narrowed could be adjusted *in situ* to achieve optimal balance between these two competing interests.

Aside from the problem of adjusting the internal circumference of body passages *in situ*, there is often a need in medicine and surgery to place a prosthetic implant at a desired recipient anatomic site. For example, existing methods proposed for percutaneous mitral repair include approaches through either the coronary sinus or percutaneous attempts to affix the anterior mitral leaflet to the posterior mitral leaflet. Significant clinical and logistical problems attend both of these existing technologies. In the case of the coronary sinus procedures, percutaneous access to the coronary sinus is technically difficult and time consuming to achieve, with procedures which may require several hours to properly access the coronary sinus. Moreover, these procedures employ incomplete annular rings, which compromise their physiologic effect. Such procedures are typically not effective for improving mitral regurgitation by more than one clinical grade. Finally, coronary sinus procedures carry the potentially disastrous risks of either fatal tears or catastrophic thrombosis of the coronary sinus.

Similarly, percutaneous procedures which employ sutures, clips, or other devices to affix the anterior mitral leaflets to the posterior mitral leaflets also have limited reparative capabilities. Such procedures are also typically ineffective in providing a complete repair of mitral regurgitation.. Furthermore, surgical experience indicates that such methods are not durable, with likely separation of the affixed valve leaflets. These procedures also fail to address the pathophysiology of the dilated mitral annulus in ischemic heart disease. As a result of the residual anatomic pathology, no ventricular remodeling or improved ventricular function is likely with these procedures.

The need exists, therefore, for a delivery system and methods for its use that would avoid the need for open surgery in such exemplary circumstances, and allow delivery, placement, and adjustment of a prosthetic implant to reduce the diameter of such a mitral annulus in a percutaneous or other minimally invasive procedure, while still achieving clinical and physiologic results that are at least the equivalent of the yields of the best open surgical procedures for these same problems.

The preceding cardiac applications are only examples of some applications according to the present invention. Another exemplary application anticipated by the present invention is in the field of gastrointestinal surgery, where the aforementioned Nissen fundoplication procedure has long been used to narrow the gastro-esophageal junction for relief of gastric reflux into the esophagus. In this setting, a surgeon is conventionally faced with the tension

between creating sufficient narrowing to achieve reflux control, but avoiding excessive narrowing that may interfere with the passage of nutrient contents from the esophagus into the stomach. Additionally, "gas bloat" may cause the inability to belch, a common complication of over-narrowing of the GE junction.

5 An adjustable prosthetic implant according to the present invention could allow *in situ* adjustment in such a setting under physiologic assessment after primary surgical closure. Such an adjustable prosthetic implant according to the present invention could be placed endoscopically, percutaneously, or with an endoscope placed within a body cavity or organ, or by trans-abdominal or trans-thoracic

10 approaches. In addition, such an adjustable prosthetic implant according to the present invention could be coupled with an adjustment means capable of being placed in the subcutaneous or other anatomic tissues within the body, such that remote adjustments could be made to the implant during physiologic function of the implant. This adjustment means can also be contained within the implant and

15 adjusted remotely, *i.e.* remote control adjustment. Such an adjustment means might be capable of removal from the body, or might be retained within the body indefinitely for later adjustment.

The present invention and the methods for its use anticipate many alternate embodiments in other potential applications in the broad fields of

20 medicine and surgery. Among the other potential applications anticipated according to the present invention are adjustable implants for use in the treatment of morbid obesity, urinary incontinence, anastomotic strictures, arterial stenosis, urinary incontinence, cervical incompetence, ductal strictures, and anal incontinence. The preceding discussions are intended to be exemplary

25 embodiments according to the present invention and should not be construed to limit the present invention and the methods for its use in any way.

SUMMARY OF THE INVENTION

In a first aspect, the present invention is directed to a novel prosthetic

30 implant and method for use for adjusting the internal circumference of an anatomic passage that can be adjusted after implantation but after the resumption of normal flow of anatomic fluids *in situ*. In another aspect, the present invention is directed to a novel delivery system and methods for its use for the delivery and placement of a prosthetic implant within an anatomic site.

35 Furthermore, the delivery system and methods according to the present invention are capable of *in situ* adjustment of such a prosthetic implant following its placement.

An adjustable prosthetic implant according to a first aspect of the present invention could allow *in situ* adjustment after initial narrowing of the

circumference of an internal anatomic passage under physiologic assessment after primary surgical closure. Such an adjustable prosthetic implant according to the present invention could be placed through an open surgical incision, or it could be placed endoscopically, either percutaneously or with an endoscope placed within a body cavity or organ. In addition, such an adjustable prosthetic implant according to the present invention could be coupled with an adjustment means capable of being placed in the subcutaneous or other anatomic tissues within the body, such that remote adjustments could be made to the implant during physiologic function of the implant. Such an adjustment means might be capable of removal from the body, or might be retained within the body indefinitely for later adjustment.

The present invention and the methods for its use anticipate many alternate embodiments in other potential applications in the broad fields of medicine and surgery. Among the other potential applications anticipated according to the present invention are adjustable implants for use in the treatment of anal incontinence, urinary incontinence, anastomotic strictures, arterial stenosis, urinary incontinence, cervical incompetence, ductal strictures, morbid obesity, and for tricuspid valvular dysfunction. The preceding discussions are intended to be exemplary embodiments according to the present invention and should not be construed to limit the present invention and the methods for its use in any way.

In another exemplary application according to the present invention, a dysfunctional cardiac valve could be replaced or functionally supplemented to relieve disease without the need for open heart surgery by a delivery system and methods for use that would allow placement of a prosthetic heart valve by a similar percutaneous or other minimally invasive procedure.

Objects, features, and advantages of the present invention will become apparent upon reading the following specification, when taken in conjunction with the drawings and the appended claims.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a front view of a first embodiment of an implant for reducing the circumference of an anatomic orifice.

FIG. 2 is a front view of the implant of **FIG. 1** secured to the annulus of a mitral valve, with the implant in an expanded position.

FIG. 3 is a front view of the implant of **FIG. 1** secured to the annulus of a mitral valve, with the implant in a contracted position to reduced the size of the heart valve opening.

FIG. 4 is a perspective view of a second embodiment of an implant for reducing the circumference of an anatomic orifice, inserted through an open operative cardiac incision and secured around the mitral valve.

FIG. 5 is a perspective view of the implant of FIG. 4, showing the cardiac incision closed, an adjustment tool extending through the closed incision, and adjustment of the implant possible after the patient has been taken "off pump."

FIG. 6 is a perspective view of a first embodiment of an adjustment means for adjusting the circumference of an implant for reducing the circumference of an anatomic orifice.

FIG. 7 is a right side view of the adjustment means of FIG. 6.

FIG. 8 is a left side view of the adjustment means of FIG. 6.

FIG. 9 is a right side view of a second embodiment of an adjustment means for adjusting the circumference of an implant for reducing the circumference of an anatomic orifice.

FIG. 10 is a perspective view of a first alternate embodiment of an attachment means for the implant of FIG. 1.

FIG. 11 is a perspective view of a second alternate embodiment of an attachment means for the implant of FIG. 1.

FIG. 12 is a perspective view of a third embodiment of an implant for reducing the circumference of an anatomic orifice.

FIG. 13 is a perspective view of one end of the implant of FIG. 12 showing an optional keyed relationship between three coaxial cannulae to prevent relative rotation between the three components.

FIG. 14 is a perspective view of the implant of FIG. 12 showing the outer cannula extended to cover the implant.

FIG. 15 is a perspective view of the implant of FIG. 12 showing the outer cannula retracted to expose the implant.

FIG. 16 is a perspective view of the implant of FIG. 12 showing the middle cannula extended to unfold the implant.

FIGS. 17 and 18 are schematic views illustrating how extension of the middle cannula causes the implant to unfold, where

FIG. 17 shows the implant in the folded position, and

FIG. 18 shows the implant in the unfolded position.

FIG. 19 is a perspective view of the lower end of a touchdown sensor of the implant of FIG. 12, showing the sensor in an uncompressed condition.

FIG. 20 is a perspective view of the lower end of the touchdown sensor of FIG. 19, showing the sensor in a compressed condition.

FIG. 21 is a perspective end view of a fourth embodiment of an implant for reducing the circumference of an anatomic orifice.

FIG. 22 is a side view of the implant of **FIG. 21** with the implant opened up to show its full length.

FIG. 23 is a side view of the adjustment mechanism of the implant of **FIG. 21**.

5 **FIG. 24** is a close-up view of two of the retention barbs of the implant of **FIG. 21**.

FIG. 25 is a front view of a fifth embodiment of an implant for reducing the circumference of an anatomic orifice, with the implant shown in its expanded configuration.

10 **FIG. 26** is a front view of the implant of **FIG. 25**, with the implant shown in its contracted configuration.

FIG. 27 is an enlarged view of the area indicated by the circle 27 in **FIG. 25**, with the outer body removed to show interior detail.

15 **FIG. 28** is a schematic view showing the implant of **FIG. 12** anatomically positioned at the mitral annulus in a heart with the implant in a fully expanded state.

FIG. 29 is a schematic view showing the implant of **FIG. 12** anatomically positioned at the gastroesophageal opening with the implant in a fully expanded state.

20 **FIG. 30** is a schematic view showing the implant of **FIG. 29** implanted to reduce the circumference of the gastroesophageal opening.

DETAILED DESCRIPTION OF THE DISCLOSED EMBODIMENT

Referring now to the drawings, in which like numerals indicate like
25 elements throughout the several views, an exemplary implant 10 comprising an implant body 15 is shown in **Fig. 1**. The implant body may be provided in a shape and size determined by the anatomic needs of an intended native recipient anatomic site within a mammalian patient. Such a native recipient anatomic site may be, by way of illustration and not by way of limitation, a heart valve, the
30 esophagus near the gastro-esophageal junction, the anus, or other anatomic sites within a mammalian body that are creating dysfunction that might be relieved by an implant capable of changing the size and shape of that site and maintaining a desired size and shape after surgery.

The implant 10 of **FIG. 1** comprises a circular implant body 15 which is
35 provided with adjustable corrugated sections 20 alternating with intervening grommet-like attachment means 25 having narrowed intermediate neck portions. As can be seen in **FIGS. 2 and 3**, the implant body 15 may be secured to the annulus of a heart valve 30 by a fixation means such as a suture 35 secured over or through the attachment means 25. The corrugated sections 20 fold and unfold

as the circumference of the implant body 15 shortens or lengthens. Adjustment of the implant 10 *in situ* may decrease the overall size of the heart valve 30, increasing the coaptation of the valve leaflets 40, and changing the configuration from that shown in FIG. 2 to that shown in FIG. 3.

5 An additional exemplary embodiment 100 of the present invention is shown in FIGS. 4 and 5, with an open operative cardiac incision 105 in a heart 110 shown in FIG. 4, and closure of the cardiac incision 105 in FIG. 5. As shown in FIG. 4, the exemplary adjustable implant 100 according to the present invention comprises an implant body 115 with attachment means 120 that allows
10 fixation to the annulus of a mitral valve 125. The exemplary adjustable implant 100 is further provided with an adjustment means 130 that is controlled by an attached or coupled adjustment tool 135. After closure of the myocardial incision 105 in FIG. 5, the adjustment tool 135 remains attached or coupled to the adjustment means 130, so that the size and shape of the implant 100 may
15 further be affected after physiologic flow through the heart 110 is resumed, but with the chest incision still open. Once the desired shape and function are achieved, the adjustment tool 135 may be disengaged from the adjustment means 130 and withdrawn from the myocardial incision 105. In various embodiments according to the present invention, the adjustment means 130 may be configured
20 and placed to allow retention by or re-introduction of the adjustment tool 135 for adjustment following closure of the chest incision.

To use the implant 100 of FIGS. 4 and 5, the physician makes the open operative incision 105 in the heart 110, as shown in FIG. 4, in the conventional manner. The implant 100, mounted at the forward end of adjustment tool 135, is
25 then advanced through the incision 105 and sutured to the annulus of the mitral valve 125. The adjustment tool 135 is then manipulated, e.g., rotated, depending upon the design of the adjustment means 130, to cause the adjustment means to reduce the size of the implant body 115, and hence the underlying mitral valve 125 to which it is sutured, to an approximate size. The myocardial incision 105
30 can now be closed, as shown in FIG. 5, leaving the adjustment tool extending through the incision for post-operative adjustment.

Once the patient has been taken "off pump" and normal flow of blood through the heart 110 has resumed, but before the chest incision has been closed, further adjustments to the size of the mitral valve 125 can be made by
35 manipulating the adjustment tool 135.

FIGS. 6-8 show an exemplary adjustment means 200 for adjusting the circumference of an annular implant such as the implant 100 previously described. The adjustment means 200 comprises a rack and pinion system in which a first cam 205 with geared teeth 210 and an engagement coupler 215

turns on a first axel 220. In this example, the first cam 205 engages a geared rack 225 on one or more surfaces of a first band 230. The first band 230 passes between the first cam 205 and a second cam 235 that turns on a second axel 240 that is joined to a second band 245. As shown in FIG. 8, the first and second
5 axels 220, 240 are maintained in suitable spaced-apart relation by means of a bracket 250 formed at the end of the second band 245.

The adjustment means 200 is preferably set within a hollow annular implant 100 of the type previously described, though it is possible to use the adjustment means in a stand-alone configuration wherein the first and second
10 bands 230, 245 are opposing ends of the same continuous annular structure. In either event, to adjust the length of an implant comprising the adjustment means 200, a tool such as a hex wrench engages the engagement coupler 215 on the first cam 205 and rotates the first cam in a counterclockwise direction as shown in FIG. 7, as indicated by the arrow 255. Rotation of the first cam 205 causes the
15 teeth 210 to drive the rack 225 to move the first band 230 toward the right, as indicated by the arrow 260 in FIG. 7. This movement of the first band tightens the circumference of the annular implant. If the physician inadvertently adjusts the implant too tight, reversing direction of the engagement coupler 215 will loosen the implant.

In various embodiments according to the present invention, the first and second bands 230, 245 may be separate structures, or they may be opposing ends of the same continuous structure. In such an embodiment, when motion is imparted to the engagement coupler 215, the first cam 205 is rotated, causing the geared teeth 210 to engage the geared rack 225, and causing the first band 230 to
20 move with respect to the second band 245 to adjust the circumference of an implant.

FIG. 9 shows a somewhat different configuration of an exemplary engagement means 300 according to the present invention, in which there is no engagement coupler, and a bracket 350 is provided on both sides of the cams to
30 maintain the first cam 315 and the second cam 320 in close approximation. In one proposed embodiment, the bracket is designed with close tolerances so as to press the first band 330 closely against the second band 345, thereby to hold the bands in fixed relative position by friction. In another proposed embodiment, the brackets 350 are fabricated from an elastic material such that the cams 315, 320
35 can be spread apart to insert the first band 330 between the cams, whereupon the cams are pulled back together with sufficient force to hold the bands 330, 345 in fixed relative position by friction. In still another proposed embodiment involving an elastic mounting arrangement between the cams 315, 320, the lower edge of the first band 330 and the upper edge of the second band 345 have

ating frictional or mechanical surfaces, whereby the cams 315, 320 can be spread apart to permit relative movement between the bands or released to clamp the bands together in fixed relation.

FIG. 10 shows an exemplary attachment means 400 for an implant according to the present invention. The attachment means 400 could be used, for example, in place of the attachment means 25 of the implant 10. The attachment means 400 takes the form of a grommet 410 comprising a wall 415 defining a lumen 420 and an attachment surface 425. Such an attachment means would be used with the implant body extending through the lumen 420 and with fixation devices such as sutures or wires either tied over or affixed through the attachment surface 425.

FIG. 11 shows another alternate embodiment of an attachment means 500 for an implant according to the present invention. The attachment means 500 could also be used, for example, in place of the attachment means 25 of the implant 10. FIG. 11 shows an attachment means 500 in the form of a hollow tube or tube segment 510 comprising a wall 515 defining a lumen 520, an outer surface 525, and an attachment tab 530. Such an attachment means would be used with the implant body extending through the lumen 520 and with fixation devices such as sutures or wires either tied or otherwise affixed over or through the attachment tab 530. Such fixation devices might be placed through holes 535 provided in the attachment tab 530. Alternately a solid attachment tab 530 might be provided, and the fixation devices might be passed through the solid tab. Modifications of these attachment means may be used in conjunction with a sutureless attachment system.

FIGS. 12–18 show another embodiment of a percutaneous annuloplasty device according to the present invention, in which an implant/delivery system array 600 includes a housing sheath 605 (not seen in FIG. 12), an actuating catheter 610 coaxially slidably mounted within the housing sheath 605, and a core catheter 615 coaxially slidably mounted within the actuating catheter 610. The core catheter has a central lumen 616 (FIG. 13). The actuating catheter 610 and core catheter 615 may be round tubular structures, or as shown in FIG. 13, either or both of the actuating and core catheters may be provided with one or more keyed ridges 618, 620 respectively to be received by one or more reciprocal slots 622, 624 within the inner lumen of either the housing sheath 605 or the actuating catheter 610, respectively. Such keyed ridges 618, 620 would limit internal rotation of an inner element within an outer element, should such restriction be desirable to maintain control of the inner contents from inadvertent displacement due to undesired rotational motion during use.

The implant/delivery system array 600 includes a distal tip 625 at the forward end of the core catheter 615. One or more radial implant support arms 630 have their distal ends 632 pivotably or bendably mounted to the core catheter 615 adjacent its distal tip 625. The proximal ends 634 of the radial
5 implant support arms 630 normally extend along the core catheter 615 but are capable of being displaced outward away from the core catheter.

One or more radial support struts 636 have their proximal ends 638 pivotably or bendably mounted to the distal end of the actuating catheter 610. The distal end 640 of each radial support strut is 636 pivotably or bendably
10 attached to a midpoint of a corresponding radial implant support arm 630. As the actuating catheter 610 is advanced with respect to the core catheter 615, the radial support struts 636 force the radial implant support arms 630 upward and outward in the fashion of an umbrella frame. Thus the actuating catheter 610, core catheter 615, radial support struts 636, and radial support arms 630 in
15 combination form a deployment umbrella 642.

A prosthetic implant 645 is releasably attached to the proximal ends 634 of the radial implant support arms 630. Around the periphery of the prosthetic implant 645 and extending proximally therefrom are a plurality of retention
20 barbs 646. In addition, one or more of the radial implant support arms 630 comprise touchdown sensors 648 whose proximal ends extend proximal to the implant 645. Extending through the central lumen 616 (FIG. 13) of the core catheter 615 in the exemplary embodiment 600 and out lateral ports 650 (FIG. 12) spaced proximally from the distal tip 625 are one or more release elements
25 660, which serve to release the implant 645 from the delivery system, and one or more adjustment elements 665 which serve to adjust the implant's deployed size and effect. Because the release elements 660 and adjustment elements 665 extend through the proximal end of the core catheter 615, as seen in FIGS. 14-
16, these elements can be directly or indirectly instrumented or manipulated by the physician. A delivery interface 670 (FIGS 12,16) is defined in this example
30 by the interaction of the deployment umbrella 642, the release elements 660, and the implant 645. In the disclosed embodiment, the release elements 660 may be a suture, fiber, or wire in a continuous loop that passes through laser-drilled bores in the implant 645 and in the radial implant support arms 630, and then passes through the length of the core catheter 615. In such an embodiment, the implant
35 645 may be released from the delivery system at a desired time by severing the release element 660 at its proximal end, outside the patient, and then withdrawing the free end of the release element 660 through the core catheter 610.

FIGS. 14–16 show the operation of the implant/delivery system array 600, in which an umbrella-like expansion of the prosthetic implant 645 is achieved by sliding movement of the housing sheath 605, the actuating catheter 610, and the core catheter 615. Referring first to FIG. 14, the housing sheath 605 is extended to cover the forward ends of the actuating catheter 610 and core catheter 615 for intravascular insertion of the implant/delivery system array 600. From this starting position, the housing sheath 605 is retracted in the direction indicated by the arrows 662. In FIG. 15 the housing sheath 605 has been retracted to expose the forward end of the actuating catheter 610 and the collapsed deployment umbrella 642. From this position the actuating catheter 610 is advanced in the direction indicated by the arrows 664. This will cause the deployment umbrellas to expand in the directions indicated by the arrows 666. FIG. 16 shows the expansion of the deployment umbrella 642 produced by distal motion of the actuating catheter 610 relative to the core catheter 615. After the implant 645 has been positioned and adjusted to the proper size, the housing sheath 605 is advanced in the direction indicated by the arrows 668 to collapse and to cover the deployment umbrella 642 for withdrawal of the device from the patient.

FIGS. 17 and 18 are schematic views illustrating the radial implant support arms 630 and the radial support struts 636 of the implant/delivery system array 600. In FIG. 17, a radial support strut 636 is pivotably attached at its proximal end 638 at a first pivotable joint 670 to the actuation catheter 610. The radial support strut 636 is attached at its distal end 640 to a second pivotable joint 672 at an intermediate point of a corresponding radial implant support arm 630. The radial implant support arm 630 is attached at its distal end 632 by a third pivotable joint 674 to the core catheter 620. FIG. 17 shows the assembly in a closed state. When the actuation catheter 610 is advanced distally over the core catheter 615, as shown by the arrows 676, the radial support strut 636 and the radial implant support arm 630 are extended by the motion at the first pivotable joint 670, the second pivotable joint 672, and the third pivotable joint 674, as shown by the arrow 678. This motion has the effect of expanding the deployment umbrella and folded implant (not shown in FIGS. 17 and 18), allowing it to achieve its greatest radial dimension, prior to engagement and implantation as previously discussed with reference to FIGS. 12–16.

FIGS. 19 and 20 show further details of the touchdown sensors 648 shown previously in FIG. 12. The touchdown sensor 648 of FIGS. 19 and 20 includes a distal segment 680, an intermediate segment 682, and a proximal segment 684. The distal segment 680 is spring-mounted, so that it is capable of slidable, telescoping displacement over the intermediate segment 682 to achieve a seamless junction with the proximal segment 684 upon maximal displacement.

When the touchdown sensor 648 is in its normal condition, the spring extends the proximal segment such that the sensor assumes the orientation shown in FIG. 19. When the implant 645 (FIG. 12) is seated against the periphery of an anatomical opening, the proximal segment 684 of the sensor 648 is compressed
5 against the distal segment 680, as shown in FIG. 20. The distal segment 680 and the proximal segment 684 are both constructed of, are sheathed by, or otherwise covered with a radio-opaque material. However, the intermediate segment 682 is not constructed or coated with such a radio-opaque material. Therefore, when the distal segment 680 is at rest, it is fully extended from the proximal segment
10 684, and the gap represented by the exposed intermediate segment 682 is visible on radiographic examination. However, when the distal segment 680 is brought to maximum closeness with the proximal segment 684, no such radio-opaque gap is radiographically visible, and the touchdown sensor is said to be "activated". This embodiment allows radiographic monitoring of the position of
15 the touchdown sensor 648 with respect to the degree of extension of the distal catheter segment 680. In the embodiment according to the present invention as shown, one or more touchdown detectors 648 are employed to ascertain that the delivery system for the prosthetic device is located in the proper position to deploy the implant into the mitral annulus. As this anatomic structure cannot be
20 directly identified on fluoroscopy or standard radiographic procedures, such precise location could be otherwise difficult. At the same time, precise localization and engagement of the mitral annulus is critical for proper implant function and safety.

Touchdown detectors within the embodiments according to the present
25 invention can have a multiplicity of forms, including the telescoping, spring-loaded, radio-opaque elements joined by a non-radio-opaque element as in the aforementioned examples. In embodiments employing magnetic resonance imaging, touchdown detectors according to the present invention may utilize metallic segments interposed by nonmetallic segments in a similar telescoping,
30 spring-loaded array. Other embodiments include a visually-evident system with telescoping, spring-loaded elements with color-coded or other visual features for procedures in which direct or endoscopic observation would be possible. Still other embodiments of touchdown detectors according to the present invention include touchdown detectors provided with microswitches at their tips, such that
35 momentary contact of sufficient pressure completes an electrical circuit and signals the activation of the touchdown detector to the operator. Still other touchdown detectors according to the present invention are provided with fiberoptic pathways for Rahmen laser spectroscopy or other spectral analytical techniques which are capable of detecting unique tissue qualities of the tissue at

the desired site for implantation. In addition, still other embodiments according to the present invention include touchdown detectors containing electrodes or other electronic sensors capable of detecting and signaling the operator when a desired electrophysiologic, impedance, or other measurable quality of the desired tissue is detected for proper implantation. Such electrophysiologic touchdown detectors may include electrical circuits that produce visual, auditory, or other signals to the operator that the detectors are activated and that the implant is in the proper position for attachment.

In yet other embodiments according to the present invention, other intracardiac or extracardiac imaging techniques including, but not limited to, intravascular ultrasound, nuclear magnetic resonance, virtual anatomic positioning systems, or other imaging techniques may be employed to confirm proper positioning of the implant, obviating the need for the touchdown sensors as previously described.

FIGS. 21–24 show an implant 700 according to one embodiment of the present invention. In this embodiment, the implant body 705 is bandlike and flexible. Through much of its length, the implant body 705 is provided with a series of retention barbs 710 which are oriented to facilitate placement, retention, and removal of the device. The implant body 705 is also provided with an adjustable section 715, which is provided in this example with a series of adjustment stops 720. The adjustment stops 720 may be slots, holes, detents, dimples, ridges, teeth, raised elements, or other mechanical features to allow measured adjustment of the implant 700 in use. In the embodiment shown in FIGS. 21–24, the adjustment stops 720 are engaged by a geared connector 725. FIG. 21 is an end view, showing the implant body 705 curved on itself, with the retention barbs 710 to the exterior, and with the adjustable section 715 passing through its engagement with the geared connector 725 and curving internally within the implant body 705 to form a closed, round structure. FIG. 23 shows details of an exemplary geared connector 725, in which a housing 730 is connected to the implant body 705. The housing 730 contains and supports a mechanical worm 740 with an attached first geared head 750 which mates with a second geared head 755. The second geared head 755 is attached to an adjustment stem 760 which is machined to receive a screwdriver-like adjustment element. The various embodiments according to the present invention may require a number of forms of adjustment elements. In the present example, the adjustment element is provided as a finely coiled wire with a distal tip machined to be received by a receiving slot in the adjustment stem 760 (not shown). The relationship between the distal tip of the adjustment element and the adjustment stem 760 is mechanically similar to a screwdriver bit and screwhead, such that

torsion imparted to the adjustment means by the operator will result in the turning of the adjustment stem 760 and second geared head 755 allows motion of the first geared head 750 and worm 740, which creates motion of the adjustable implant section 715 as the worm engages with the series of adjustment tops 725. Excess length of the adjustable section 715 passes through a band slot 735 (FIG. 23), thus allowing the band to move concentrically inside the closed implant body 705. The adjustment element in this embodiment may be designed to remain in place after the deployment umbrella has been retracted and withdrawn. The connection between the adjustment element's distal tip and the adjustment stem 760 may be a simple friction connection, a mechanical key/slot formation, or may be magnetically or electronically maintained.

As further shown in FIG. 21, the exemplary embodiment employs unidirectional retention barbs 710 which are attached to the outer perimeter of the implant body 705. The retention barbs 710 are oriented in a consistent, tangential position with respect to the implant body 705 such that rotational motion of the implant body will either engage or release the retention barbs 710 upon contact with the desired tissue at the time of deployment. This positioning of the retention barbs 710 allows the operator to "screw in" the implant 700 by turning the implant 700 upon its axis, thus engaging the retention barbs 710 into the adjacent tissue. As shown in FIG. 24, the retention barbs 710 may each be further provided with a terminal hook 775 at the end which would allow for smooth passage through tissue when engaging the retention barbs 710 by rotating the implant 700, without permitting the implant 700 to rotate in the opposite direction, because of the action of the terminal hooks 775 grasping the surrounding tissue (much like barbed fish hooks). The terminal hooks 775 thus ensure the seating of the implant 700 into the surrounding tissue.

FIGS. 25-27 illustrate another embodiment of an implant 800 as contemplated according to the present invention. The implant 800 includes a band 805 (FIG. 27), but the retention barbs of the previous example have been eliminated in favor of an outer fabric implant sheath 810. The fabric sheath 810 can be sutured or otherwise affixed to the anatomic tissue in a desired location. The circumference of the implant body 800 is adjusted through a geared connector 825 similar to the geared connector of the bandlike implant array shown in FIG. 23. More specifically, adjustment stops 820 on the band are engaged by a mechanical worm 840 with an attached first geared head 850. The first geared head 850 mates with a second geared head 855. The second geared head 855 is attached to an adjustment stem 860 which is machined to receive a screwdriver-like adjustment element.

FIG. 28 illustrates an example of the method of use of an implant/delivery system array 600 for positioning an implant 645 in a patient with ischemic annular dilatation and mitral regurgitation. Peripheral arterial access is obtained via conventional cutdown, arterial puncture, or other standard access techniques.

5 After access to the arterial system is attained, guidewire placement is performed and intravascular access to the heart 900 is obtained using fluoroscopic, ultrasound, three-dimension ultrasound, magnetic resonance, or other real-time imaging techniques. The guidewire, deployment device, and implant are passed through the aortic valve in a retrograde fashion into the left ventricle 905 and

10 then into the left atrium 910. At this point, the operator retracts the housing sheath 605, thus unsheathing the collapsed deployment umbrella 642 and implant 645. The deployment umbrella 642 is then distended by the distal motion of the actuation catheter, causing the radial support arms and struts to fully distend. At this point, the touchdown detectors 648 are not in contact with

15 any solid structures, and are fully extended with their radiolucent gaps visible on the imaging system. Once the deployment umbrella is distended, the entire assembly is pulled back against the area of the mitral valve 915. At least two touchdown detectors 648 are employed in a preferred embodiment according to the present invention. When all touchdown detectors show the disappearance of

20 their intermediate, non-opaque, intermediate segments and are thus activated, then the deployment umbrella must be in contact with the solid tissue in the region of the mitral annulus/atrial tissue, and further implant deployment and adjustment may proceed. However, if any one touchdown sensor is not activated, and a radiolucent gap persists, then the device is not properly positioned, and

25 must be repositioned before further deployment. Thus, the touchdown sensor system may assist in the deployment and adjustment of prosthetic devices by the delivery system according to the present invention. Once properly positioned, the operator rotates the actuation catheter in a prescribed clockwise or counterclockwise manner to engage the retention barbs on the implant into the

30 tissue in the region of the mitral annulus/atrial tissue. Should re-positioning be required, a reverse motion would disengage the retention barbs from the annular/atrial tissue, and repositioning may be performed, again using the touchdown detectors for proper placement. Once firmly seated, the adjustment element(s) are operated to achieve the desired degree of annular reduction. Real-

35 time trans esophageal echocardiography, intravascular echocardiography, intracardiac echocardiography, or other modalities for assessing mitral function may then be employed to assess the physiologic effect of the repair on mitral function, and additional adjustments may be performed. Once a desired result has been achieved, the release elements are activated to detach the implant from

the deployment umbrella. The operator then retracts the actuation catheter and extends the housing sheath, collapsing the deployment umbrella and covering the components for a smooth and atraumatic withdrawal of the device from the heart and vascular system.

5 If desired, the adjustment elements may be left in position after the catheter components are withdrawn for further physiologic adjustment. In yet other embodiments according to the present invention, a catheter-based adjustment elements may subsequently be re-inserted through a percutaneous or other route. Such an adjustment element may be steerably operable by the
10 operator, and may be provided with magnetic, electronic, electromagnetic, or laser-guided systems to allow docking of the adjustment element with the adjustable mechanism contained within the implant. In still other embodiments, the adjustment mechanism may be driven by implanted electromechanical motors or other systems, which may be remotely controlled by electronic flux or
15 other remote transcutaneous or percutaneous methods.

In the case of pulmonic valve repair, initial catheter access is achieved through a peripheral or central vein. Access to the pulmonary valve is also achieved from below the valve once central venous access is achieved by traversing the right atrium, the tricuspid valve, the right ventricle, and
20 subsequently reaching the pulmonic valve.

In yet other embodiments according to the present invention, catheter access to the left atrium can be achieved from cannulation of central or peripheral veins, thereby achieving access to the right atrium. Then a standard atrial trans-septal approach may be utilized to access the left atrium by creation
25 of an iatrogenic atrial septal defect (ASD). In such a situation, the mitral valve may be accessed from above the valve, as opposed to the retrograde access described in Example 1. The implant and a reversed deployment umbrella may be utilized with implant placement in the atrial aspect of the mitral annulus, with the same repair technique described previously. The iatrogenic ASD may then be
30 closed using standard device methods. Access to the aortic valve may also be achieved from above the aortic valve via arterial access in a similar retrograde fashion.

Other embodiments of the adjustable implant and methods according to the present invention include gastrointestinal disorders such as gastro-
35 esophageal reflux disease (GERD), a condition in which the gastro-esophageal (GE) junction lacks adequate sphincter tone to prevent the reflux of stomach contents into the esophagus, causing classic heartburn or acid reflux. This not only results in discomfort, but may cause trauma to the lower esophagus over time that may lead to the development of pre-cancerous lesions (Barrett's

esophagus) or adenocarcinoma of the esophagus at the GE junction. Surgical repair of the GE junction has historically been achieved with the Nissen Fundoplication, an operative procedure with generally good results. However, the Nissen procedure requires general anesthesia and a hospital stay. Utilizing
5 the devices and methods according to the present invention, an adjustable implant would obviate the need for a hospital stay and be performed in a clinic or gastroenterologist's office. Referring now to FIGS. 29 and 30, an umbrella deployment device 600 with implant 645 is passed under guidance of an endoscope 1000, through the patient's mouth, esophagus 1005, and into the
10 stomach 1010, where the deployment device 600 is opened with expansion of the implant 645 and touchdown detectors 648 with a color-coded or otherwise visible gap. The touchdown detectors are then engaged onto the stomach around the gastroesophageal junction 1015 under direct endoscopic control until all touchdown detectors 648 are visually activated. The implant is then attached to
15 the stomach wall, 1020 the umbrella 642 is released and withdrawn, leaving behind the implant 645 and the adjustment elements. The implant is then adjusted until the desired effect is achieved, i.e., minimal acid reflux either by patient symptoms, pH monitoring of the esophagus, imaging studies, or other diagnostic means. If the patient should suffer from gas bloat, a common
20 complication of gastroesophageal junction repair in which the repair is too tight and the patient is unable to belch, the implant can be loosened until a more desirable effect is achieved.

In various embodiments anticipated by the present invention, the implant body may be straight, curved, circular, ovoid, polygonal, or some combination
25 thereof. In various embodiments anticipated by the present invention the implant may be capable of providing a uniform or non-uniform adjustment of an orifice or lumen within the body. The implant body may further completely enclose the native recipient anatomic site, or it may be provided in an interrupted form that encloses only a portion of the native recipient anatomic site. In still other
30 embodiments of the present invention, the implant body may be a solid structure, while in yet other embodiments the implant body may form a tubular or otherwise hollow structure. In one embodiment of the present invention, the body may further be a structure with an outer member, an inner member, and optional attachment members. In such an embodiment, the outer member of the
35 implant body may serve as a covering for the implant, and is designed to facilitate and promote tissue ingrowth and biologic integration to the native recipient anatomic site. The outer member in such an embodiment may be fabricated of a biologically compatible material, such as Dacron, PTFE, malleable metals, other biologically compatible materials or a combination of

such biologically compatible materials in a molded, woven, or non-woven configuration. The outer member in such an embodiment also serves to house the inner member. In this embodiment, the inner member provides an adjustment means that, when operated by an adjustment mechanism, is capable of altering the shape and/or size of the outer member in a defined manner.

In alternate embodiments according to the present invention, the adjustment means may be located external to or incorporated within the outer member. In yet additional alternate embodiments contemplated by the present invention, the implant body may consist of an adjustment means without a separate outer member covering said adjustment means.

In various embodiments according to the present invention, the adjustment means may include a mechanism which may be threaded or non-threaded, and which may be engaged by the action of a screw or worm screw, a friction mechanism, a friction-detent mechanism, a toothed mechanism, a ratchet mechanism, a rack and pinion mechanism, or such other devices to permit discreet adjustment and retention of desired size a desired position, once the proper size is determined.

In yet other embodiments according to the present invention, the adjustment means may comprise a snare or purse string-like mechanism in which a suture, a band, a wire or other fiber structure, braided or non-braided, monofilament or multifilament, is capable of affecting the anatomic and/or physiologic effects of the implant device on a native anatomic recipient site upon varying tension or motion imparted to said wire or fiber structure by a surgeon or other operator. Such an adjustment means may be provided as a circular or non-circular structure in various embodiments. Changes in tension or motion may change the size and/or shape of the implant.

In various embodiments according to the present invention, the adjustment means may be a metallic, plastic, synthetic, natural, biologic, or any other biologically-compatible material, or combination thereof. Such adjustment means may further be fabricated by extrusion or other molding techniques, machined, or woven. Furthermore, in various embodiments of the present invention, the adjustment means may be smooth or may include slots, beads, ridges, or any other smooth or textured surface.

In various embodiments of the present invention, the implant body may be provided with one or more attachment members such as grommets or openings or other attachment members to facilitate attachment of the implant to the native recipient site. In alternate embodiments, the implant body may attach to or incorporate a mechanical tissue interface system that allows a sutureless mechanical means of securing the implant at the native recipient site. In still

other alternate embodiments, sutures or other attachment means may be secured around or through the implant body to affix the implant body to the native recipient site. In yet other embodiments of the present invention, mechanical means of securing the implant body to the native recipient site may be augmented or replaced by use of fibrin or other biologically-compatible tissue
5 glues or similar adhesives.

In additional various embodiments according to the present invention, the adjustable implant may be employed to adjustably enlarge or maintain the circumference or other dimensions of an orifice, ostium, lumen, or anastomosis
10 in which a disease process tends to narrow or constrict such circumference or other dimensions.

In various embodiments according to the present invention, an adjustment mechanism may be provided to interact with the adjustment means to achieve the desired alteration in the size and/or position of the adjustment means. Such
15 an adjustment mechanism may include one or more screws, worm-screw arrays, rollers, gears, frictional stops, a friction-detent system, ratchets, rack and pinion arrays, micro-electromechanical systems, other mechanical or electromechanical devices or some combination thereof.

In some embodiments as contemplated by the present invention, an adjustment tool may be removably or permanently attached to the adjustment
20 mechanism and disposed to impart motion to the adjustment mechanism and, in turn, to the adjustment means to increase or decrease the anatomic effect of the implant on the native recipient site.

In alternate embodiments according to the present invention, micromotor arrays with one or more micro-electromechanical motor systems with related
25 electronic control circuitry may be provided as an adjustment means, and may be activated by remote control through signals convey by electromagnetic radiation or by direct circuitry through electronic conduit leads which may be either permanently or removably attached to said micromotor arrays.

In still other various embodiments according to the present invention, the adjustment mechanism may be provided with a locking mechanism disposed to
30 maintain the position of the adjustment means in a selected position upon achievement of the optimally desired anatomic and/or physiologic effect upon the native recipient site and the bodily organ to which it belongs. In other
35 embodiments, no special locking mechanism may be necessary due to the nature of the adjustment means employed.

In yet other alternate embodiments according to the present invention, the adjustment means and/or the outer member structure may be a pliable synthetic material capable of rigidification upon exposure to electromagnetic radiation of

selected wavelength, such as ultraviolet light. In such embodiments, exposure to the desired electromagnetic radiation may be achieved by external delivery of such radiation to the implant by the surgeon, or by internal delivery of such radiation within an outer implant member using fiberoptic carriers placed within said outer member and connected to an appropriate external radiation source. Such fiberoptic carriers may be disposed for their removal in whole or in part from the outer implant member after suitable radiation exposure and hardening of said adjustment means.

The present invention also provides methods of using an adjustable implant device to selectively alter the anatomic structure and/or physiologic effects of tissues forming a passageway for blood, other bodily fluids, nutrient fluids, semi-solids, or solids, or wastes within a mammalian body. Various embodiments for such uses of adjustable implants include, but are not limited to, open surgical placement of said adjustable implants at the native recipient site through an open surgical incision, percutaneous or intravascular placement of said implants under visual control employing fluoroscopic, ultrasound, magnetic resonance imaging, or other imaging technologies, placement of said implants through tissue structural walls, such as the coronary sinus or esophageal walls, or methods employing some combination of the above techniques. In various embodiments as contemplated by the present invention, adjustable implants may be placed and affixed in position in a native recipient anatomic site by trans-atrial, trans-ventricular, trans-arterial, trans-venous (i.e., via the pulmonary veins) or other routes during beating or non-beating cardiac surgical procedures or endoscopically or percutaneously in gastrointestinal surgery.

Furthermore, alternate methods for use of an adjustable implant device may provide for the periodic, post-implantation adjustment of the size of the anatomic structure receiving said implant device as needed to accommodate growth of the native recipient site in a juvenile patient or other changes in the physiologic needs of the recipient patient.

Adjustment of the adjustable implants and the methods for their use as disclosed herein contemplates the use by the surgeon or operator of diagnostic tools to provide an assessment of the nature of adjustment needed to achieve a desired effect. Such diagnostic tools include, but are not limited to, transesophageal echocardiography, echocardiography, diagnostic ultrasound, intravascular ultrasound, virtual anatomic positioning systems integrated with magnetic resonance, computerized tomographic, or other imaging technologies, endoscopy, mediastinoscopy, laparoscopy, thoracoscopy, radiography, fluoroscopy, magnetic resonance imaging, computerized tomographic imaging,

intravascular flow sensors, thermal sensors or imaging, remote chemical or spectral analysis, or other imaging or quantitative or qualitative analytic systems.

In one aspect, the implant/delivery system of the present invention comprises a collapsible, compressible, or distensible prosthetic implant and a delivery interface for such a prosthetic implant that is capable of delivering the prosthetic implant to a desired anatomic recipient site in a collapsed, compressed, or non-distended state, and then allowing controlled expansion or distension and physical attachment of such a prosthetic implant by a user at the desired anatomic recipient site. Such a system permits the delivery system and prosthetic implant to be introduced percutaneously through a trocar, sheath, via Seldinger technique, needle, or endoscopically through a natural bodily orifice, body cavity, or region and maneuvered by the surgeon or operator to the desired anatomic recipient site, where the delivery system and prosthetic implant may be operably expanded for deployment. When desirable, the implant/delivery system according to the present invention is also capable of allowing the user to further adjust the size or shape of the prosthetic implant once it has been attached to the desired anatomic recipient site. The delivery system according to the present invention is then capable of detaching from its interface with the prosthetic implant and being removed from the anatomic site by the operator. The delivery system and prosthetic implant may be provided in a shape and size determined by the anatomic needs of an intended native recipient anatomic site within a mammalian patient. Such a native recipient anatomic site may be a heart valve, the esophagus near the gastro-esophageal junction, the anus, or other anatomic sites within a mammalian body that are creating dysfunction that might be relieved by an implant capable of changing the size and shape of that site and maintaining a desired size and shape after surgery.

In various embodiments contemplated by the present invention, the delivery system may be a catheter, wire, filament, rod, tube, endoscope, or other mechanism capable of reaching the desired recipient anatomic site through an incision, puncture, trocar, or through an anatomic passageway such as a vessel, orifice, or organ lumen, or trans-abdominally or trans-thoracically. In various embodiments according to the present invention, the delivery system may be steerable by the operator. The delivery system may further have a delivery interface that would retain and convey a prosthetic implant to the desired recipient anatomic site. Such a delivery interface may be operably capable of distending, reshaping, or allowing the independent distension or expansion of such a prosthetic implant at the desired recipient anatomic site. Furthermore, such a delivery interface may provide an operable means to adjust the distended or expanded size, shape, or physiologic effect of the prosthetic implant once said

implant has been attached *in situ* at the desired recipient anatomic site. In various embodiments according to the present invention, such adjustment may be carried out during the procedure in which the implant is placed, or at a subsequent time. Depending upon the specific anatomic needs of a specific application, the delivery interface and the associated prosthetic implant may be straight, curved, circular, helical, tubular, ovoid, polygonal, or some combination thereof. In still other embodiments of the present invention, the prosthetic implant may be a solid structure, while in yet other embodiments the prosthetic implant may form a tubular, composite, or otherwise hollow structure. In one embodiment of the present invention, the prosthetic implant may further be a structure with an outer member, an inner member, and optional attachment members. In such an embodiment, the outer member of the prosthetic implant may serve as a covering for the implant, and is designed to facilitate and promote tissue ingrowth and biologic integration to the native recipient anatomic site. The outer member in such an embodiment may be fabricated of a biologically compatible material, such as Dacron, PTFE, malleable metals, other biologically compatible materials or a combination of such biologically compatible materials in a molded, woven, or non-woven configuration. The outer member in such an embodiment also serves to house the inner member. In this embodiment, the inner member provides an adjustment means that, when operated by an adjustment mechanism, is capable of altering the shape and/or size of the outer member in a defined manner.

In some embodiments according to the present invention, at least some portions of the adjustable inner or outer member may be elastic to provide an element of variable, artificial muscle tone to a valve, sphincter, orifice, or lumen in settings where such variability would be functionally valuable, such as in the treatment of rectal incontinence or vaginal prolapse.

In various embodiments according to the present invention, the delivery interface would have an attachment means to retain and convey the prosthetic implant en route to the native anatomic recipient site and during any *in situ* adjustment of the prosthetic implant once it has been placed by the operator. Such an attachment means would be operably reversible to allow detachment of the prosthetic implant from the delivery interface once desired placement and adjustment of the prosthetic implant has been accomplished.

Finally, it will be understood that the preferred embodiment has been disclosed by way of example, and that other modifications may occur to those skilled in the art without departing from the scope and spirit of the appended claims.

CLAIMS

What is claimed is:

- 5 1. An implantable device for controlling the internal circumference of an anatomic orifice or lumen, comprising:
 an annular ring;
 means by which said annular ring can be fastened to the tissue around an anatomic orifice or lumen;
10 means associated with said annular ring for permitting adjustment of the circumference of said annular ring from a first circumference to a second circumference; and
 means associated with said annular ring for maintaining said ring in said first circumference and, upon said annular ring being adjusted to said
15 second circumference, for maintaining said annular ring in said second circumference;
 whereby the circumference of said anatomic orifice or lumen can be adjusted by adjusting the circumference of said annular ring from said first circumference to said second circumference.
- 20 2. The implantable device of Claim 1, wherein said means by which said annular ring can be fastened to the tissue around an anatomic orifice or lumen comprises a plurality of barbs extending from said annular ring for engaging the tissue around said anatomic orifice or lumen.
- 25 3. The implantable device of Claim 2, wherein each of said barbs is oriented in a consistent, tangential direction with respect to the annular ring such that rotational motion of the annular ring in a first direction will engage said retention barbs with the desired tissue, and rotational motion of the annular ring
30 in a direction opposite to said first direction will disengage said retention barbs from said desired tissue.
4. The implantable device of Claim 3, wherein each of said barbs further comprises a hook at its free end.

35

5 5. The implantable device of Claim 1, wherein said means by which said annular ring can be fastened to the tissue around an anatomic orifice or lumen comprises an outer fabric sheath covering said annular ring through which sutures can be placed to suture said implantable device to said tissue around said anatomic orifice or lumen.

10 6. The implantable device of Claim 1, wherein said means by which said annular ring can be fastened to the tissue around an anatomic orifice or lumen comprises a plurality of grommets spaced around the periphery of said annular ring.

15 7. The implantable device of Claim 6, wherein said grommets have narrowed intermediate neck portions around which sutures can be placed and then through the underlying tissue to anchor said annular ring to the tissue around said anatomic orifice or lumen.

20 8. The implantable device of Claim 6, wherein said grommets are comprised of a material which is sufficiently soft that a suture can be placed through said grommet and through the underlying tissue to anchor said annular ring to the tissue around said anatomic orifice or lumen.

25 9. The implantable device of Claim 6, wherein said grommets comprise tabs comprised of a material which is sufficiently soft that a suture can be placed through said tab and through the underlying tissue to anchor said annular ring to the tissue around said anatomic orifice or lumen.

30 10. The implantable device of Claim 6, wherein said grommets comprise tabs, and wherein said tabs define holes through which a suture can be placed and then through the underlying tissue to anchor said annular ring to the tissue around said anatomic orifice or lumen.

35 11. The implantable device of Claim 1, wherein said means associated with said annular ring for permitting adjustment of the circumference of said annular ring from a first circumference to a second circumference comprises corrugations.

12. The implantable device of Claim 6, wherein said device comprises alternating sections of corrugations and grommets spaced around the periphery of said annular ring.

13. The implantable device of Claim 1,
wherein said annular ring comprises a hollow tube formed into an annular
shape, said tube having interspaced smooth and corrugated sections
disposed around its circumference,
5 wherein said means by which said annular ring can be fastened to the
tissue around an anatomic orifice or lumen comprises said tube being
sufficiently soft such that a suture can be passed through said tube and
hence through the underlying tissue;
10 wherein said means associated with said annular ring for permitting
adjustment of the circumference of said annular ring from a first
circumference to a second circumference comprises said corrugated
sections; and
wherein said means associated with said annular ring for maintaining said
15 ring in said first circumference and, upon said annular ring being
adjusted to said second circumference, for maintaining said annular ring
in said second circumference comprises said corrugated sections being
sufficiently stiff that once said annular ring is placed in a given
configuration, it will tend to remain in said given configuration when
20 acted upon by normal anatomic forces at said selected anatomic orifice
or lumen.

14. The implantable device of Claim 1,
wherein said annular ring comprises a hollow tube formed into an annular
25 shape, said tube having interspaced smooth and corrugated sections
disposed around its circumference,
wherein said means by which said annular ring can be fastened to the
tissue around an anatomic orifice or lumen comprises said tube having
portions of narrowed circumference such that a suture can be passed
30 around said tube at said portions of narrowed circumference and hence
through the underlying tissue;
wherein said means associated with said annular ring for permitting
adjustment of the circumference of said annular ring from a first
circumference to a second circumference comprises said corrugated
35 sections; and

wherein said means associated with said annular ring for maintaining said ring in said first circumference and, upon said annular ring being adjusted to said second circumference, for maintaining said annular ring in said second circumference comprises said corrugated sections being sufficiently stiff that once said annular ring is placed in a given configuration, it will tend to remain in said given configuration when acted upon by normal anatomic forces at said selected anatomic orifice or lumen.

10 15. The implantable device of Claim 1, wherein said means associated with said annular ring for permitting adjustment of the circumference of said annular ring from a first circumference to a second circumference comprises:

teeth formed on at least a portion of said annular ring;
a gear engaging said teeth of said annular ring; and
15 said gear and said teeth being arranged such that turning said gear effects relative movement between a first end of said annular ring and a second end of said annular ring to adjust the circumference of said annular ring from a first circumference to a second circumference.

20 16. The implantable device of Claim 15, further comprising a wheel positioned tangentially to said gear such that said portion of said annular ring which engages said gear passes between said gear and said wheel.

25 17. The implantable device of Claim 15, wherein said gear is mounted in fixed relation to said second end of said annular ring, and wherein said teeth are formed adjacent said first end of said annular ring.

30 18. The implantable device of Claim 15, further comprising means for turning said gear from a location remote from said gear, such that said circumference of said implant can be adjusted after closure of surgical incisions and resumption of physiological flow through said orifice or lumen.

35 19. The implantable device of Claim 18, wherein said means for turning said gear from a remote location is disengageable from said gear after completion of adjustments.

20. The implantable device of Claim 1, wherein said means associated with said annular ring for permitting adjustment of the circumference of said annular ring from a first circumference to a second circumference comprises:

a worm gear; and
means operatively associated with a first end of said annular ring for
engaging said worm gear such that rotation of said worm gear effects
relative movement between said first end of said annular ring and a
5 second end of said annular ring to adjust the circumference of said
annular ring from a first circumference to a second circumference.

21. The implantable device of Claim 20, wherein said worm gear has a
first angled gear head at its driven end, and further comprising a shaft in offset
10 relation to said worm gear and having a second angled gear head at a first end
thereof, said first and second angled gear heads drivably engaging such that
rotation of said shaft drives said worm gear.

22. The implantable device of Claim 21, further comprising means for
15 turning said shaft from a location remote from said worm gear, such that said
circumference of said implant can be adjusted after closure of surgical incisions
and resumption of physiological flow through said orifice or lumen.

23. The implantable device of Claim 22, wherein said shaft and said
20 means for turning said shaft from a remote location are disengageable from said
worm gear after completion of adjustments.

1/11

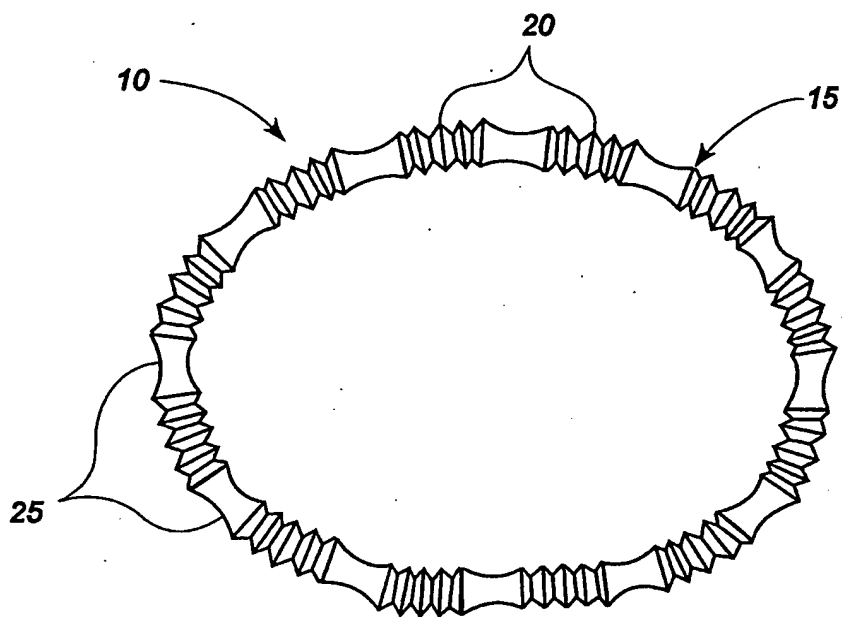


Fig. 1

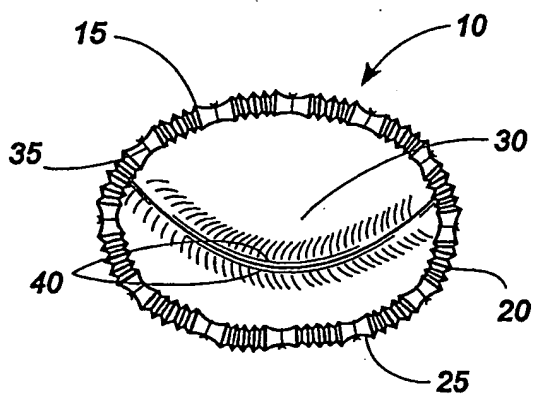


Fig. 2









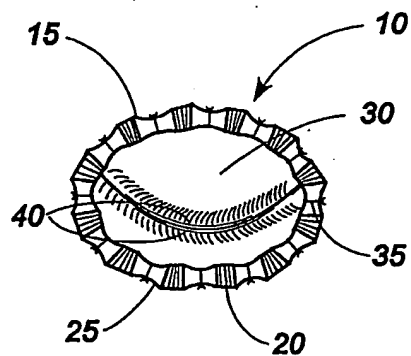


Fig. 3

2/11

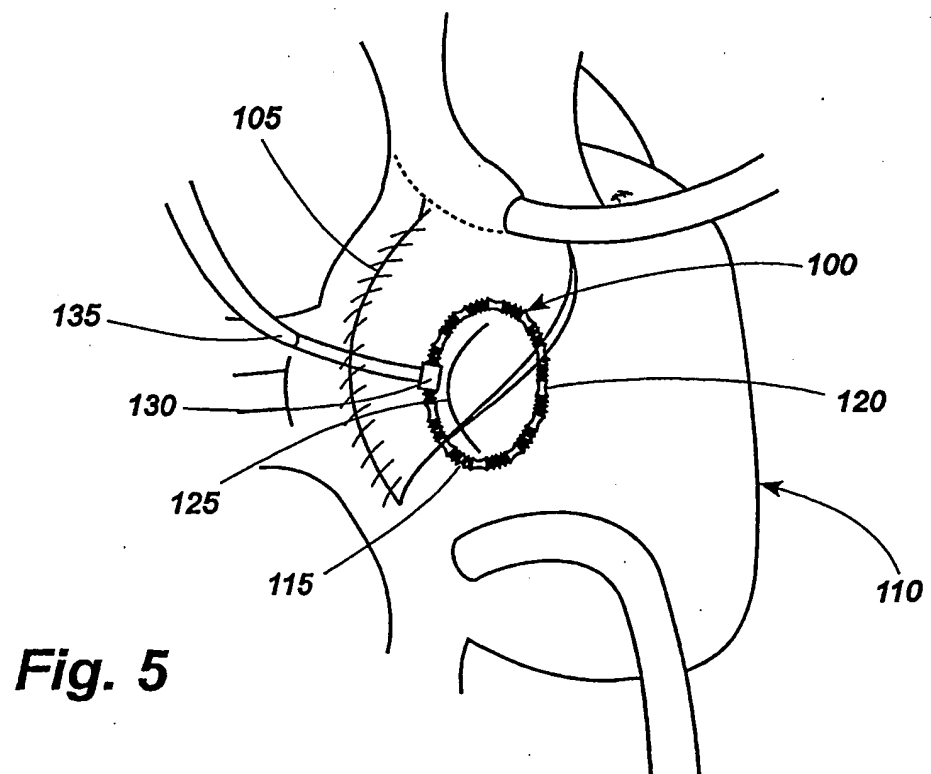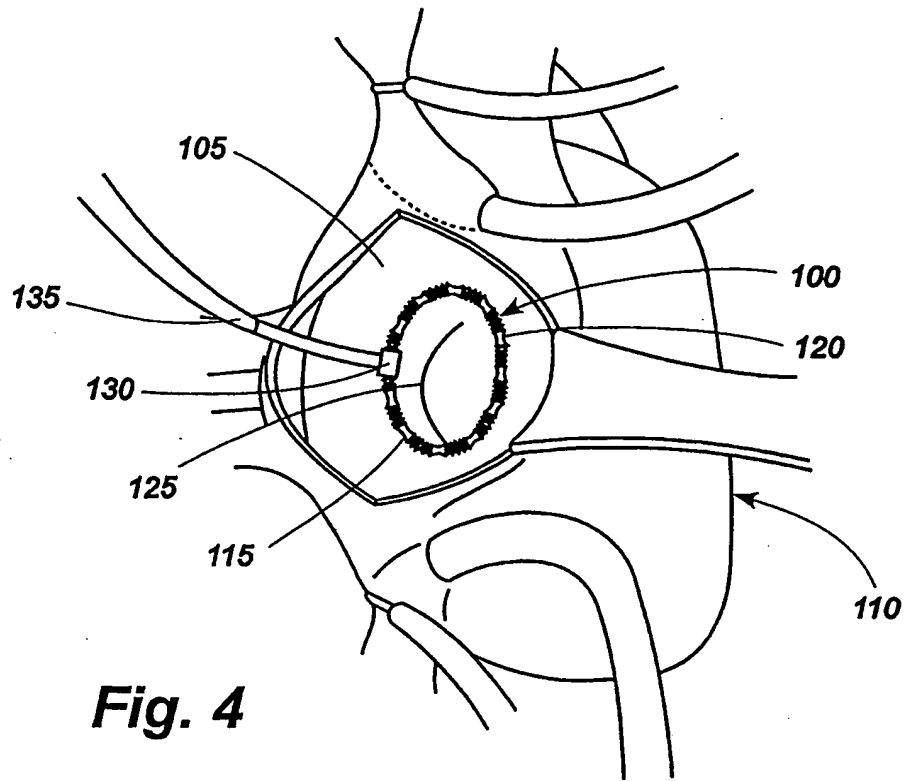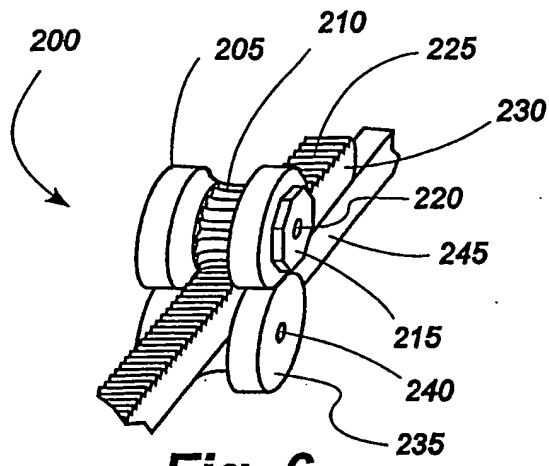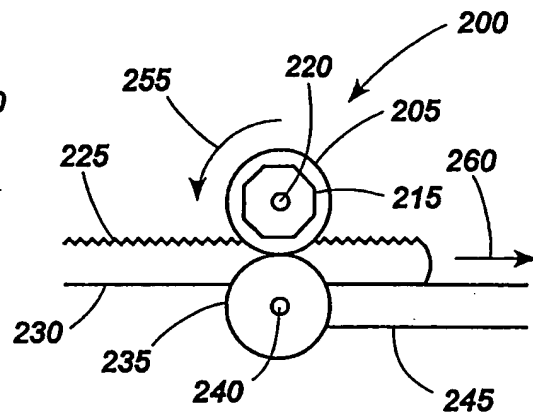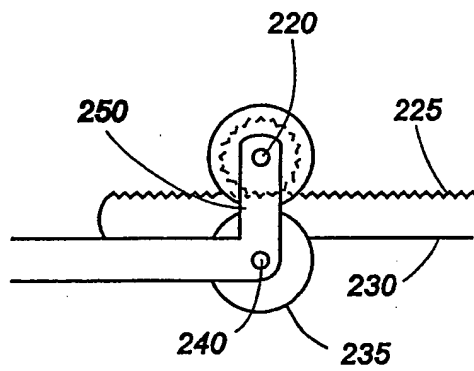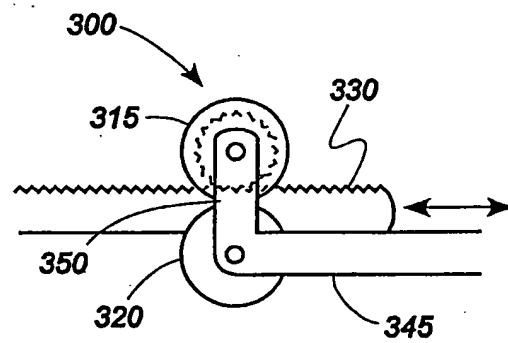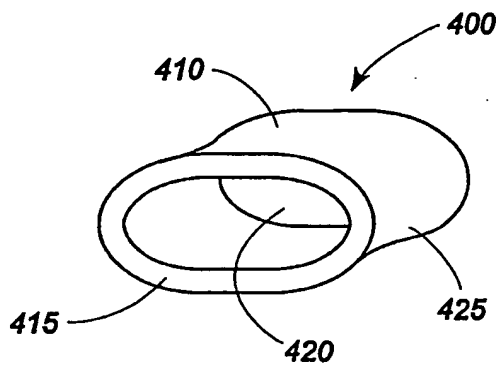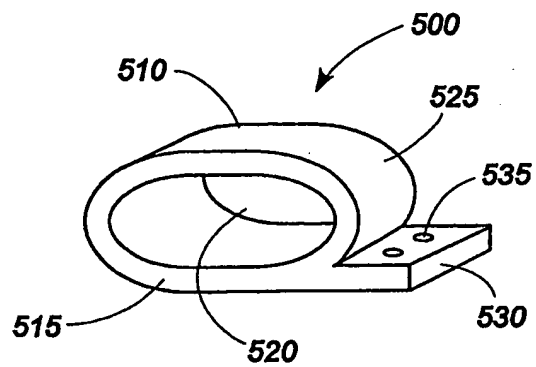

3/11

**Fig. 6****Fig. 7****Fig. 8****Fig. 9****Fig. 10****Fig. 11**

4/11

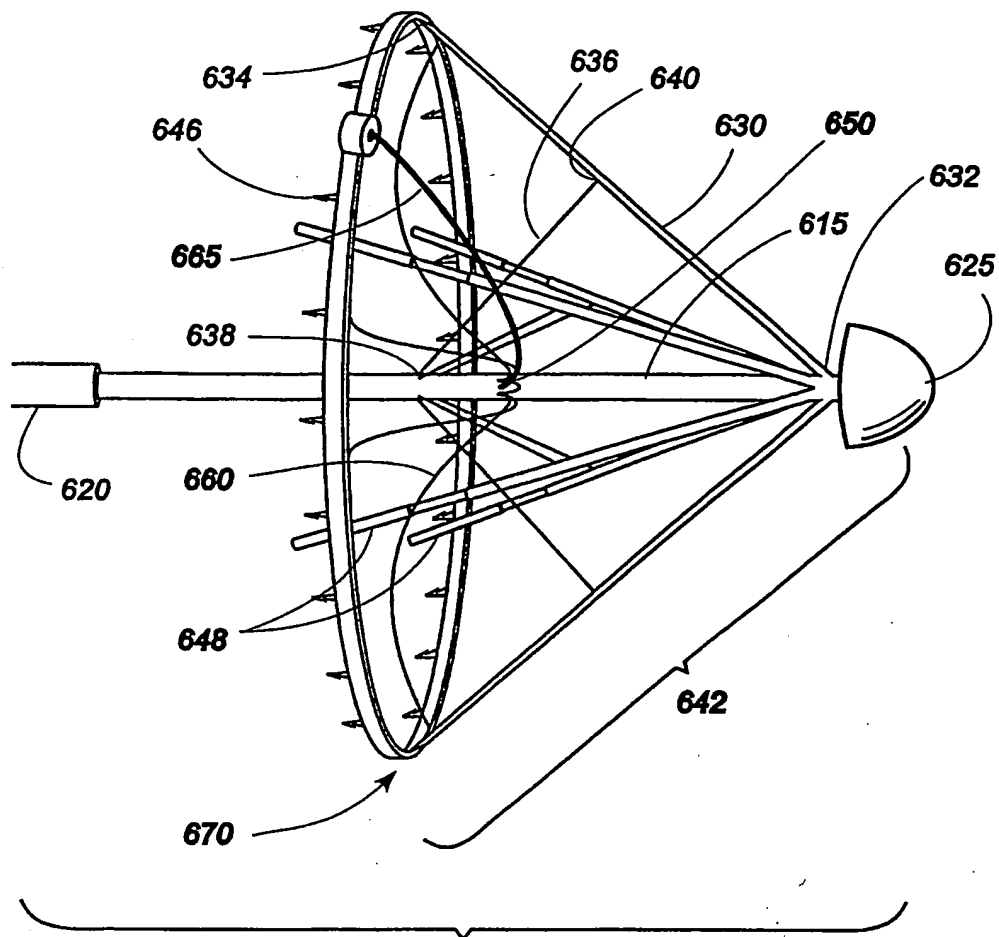


Fig. 12

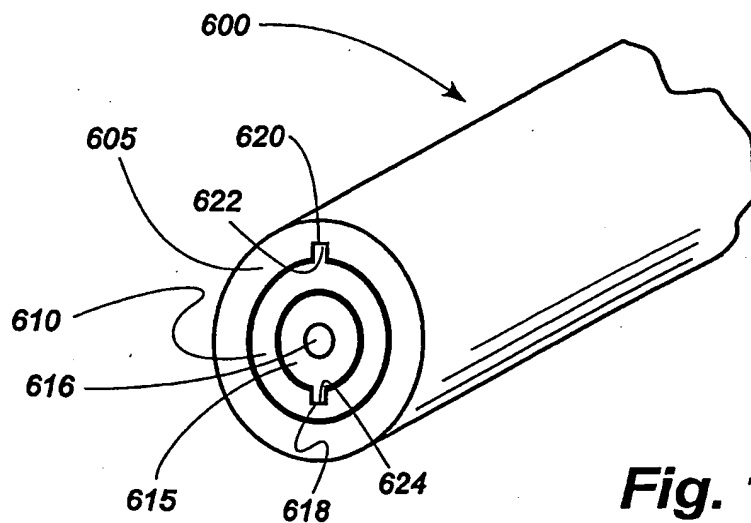


Fig. 13

5/11

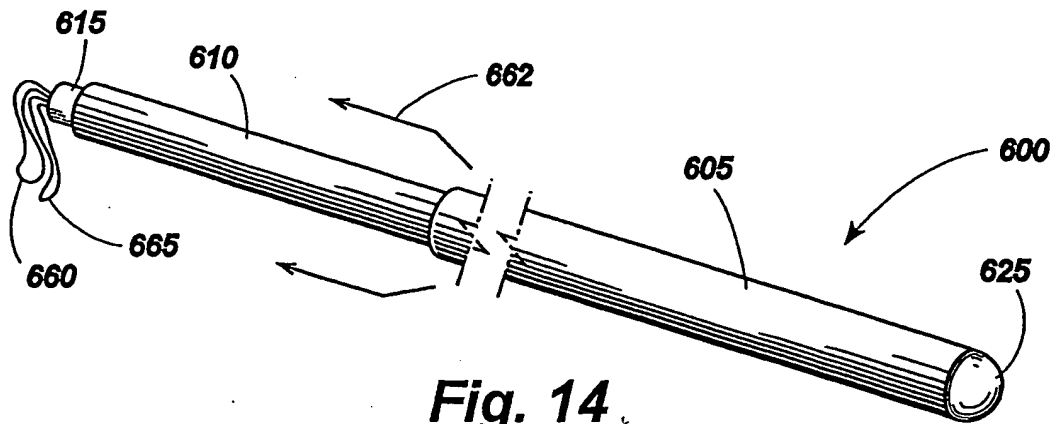


Fig. 14

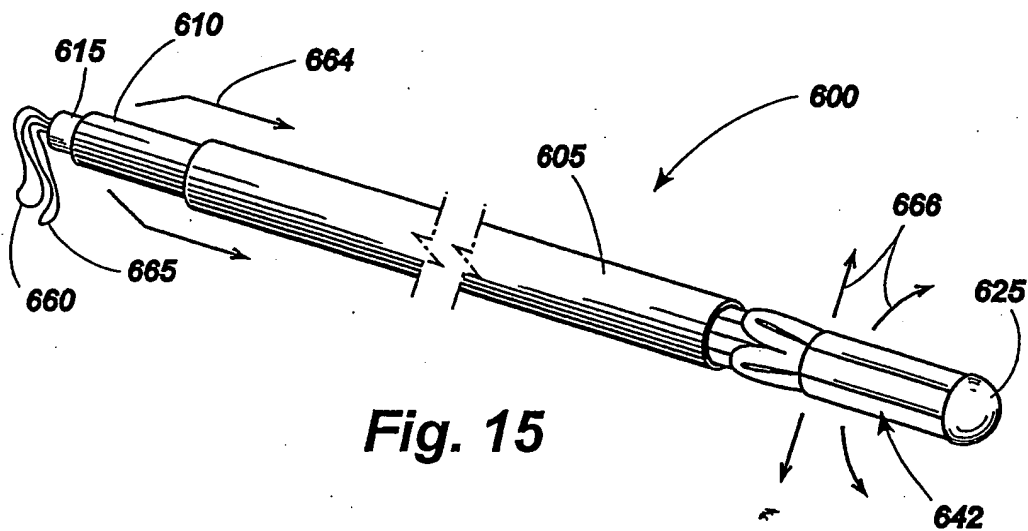


Fig. 15





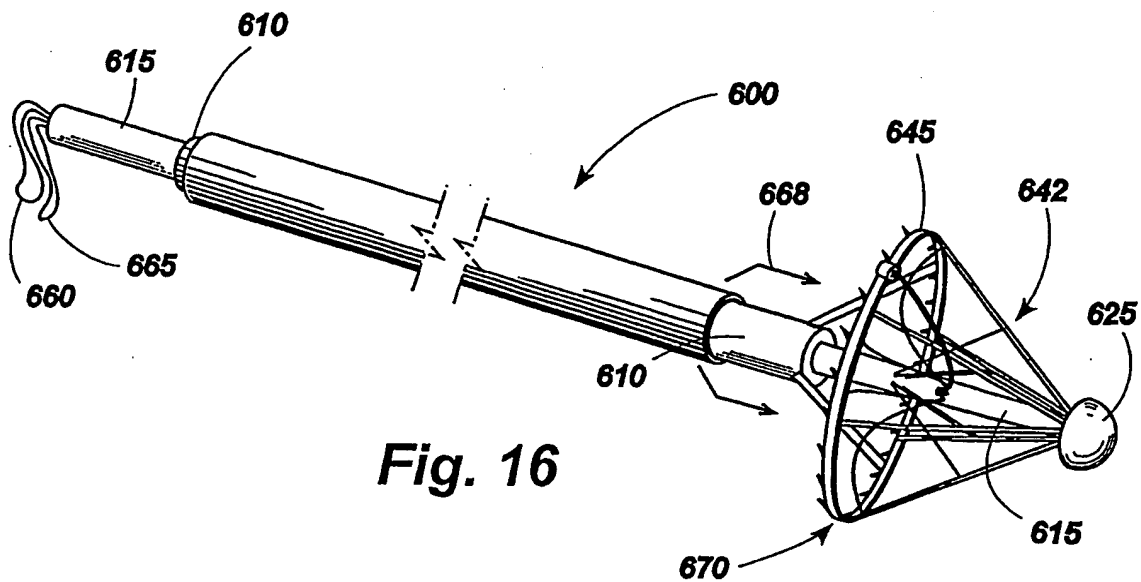


Fig. 16

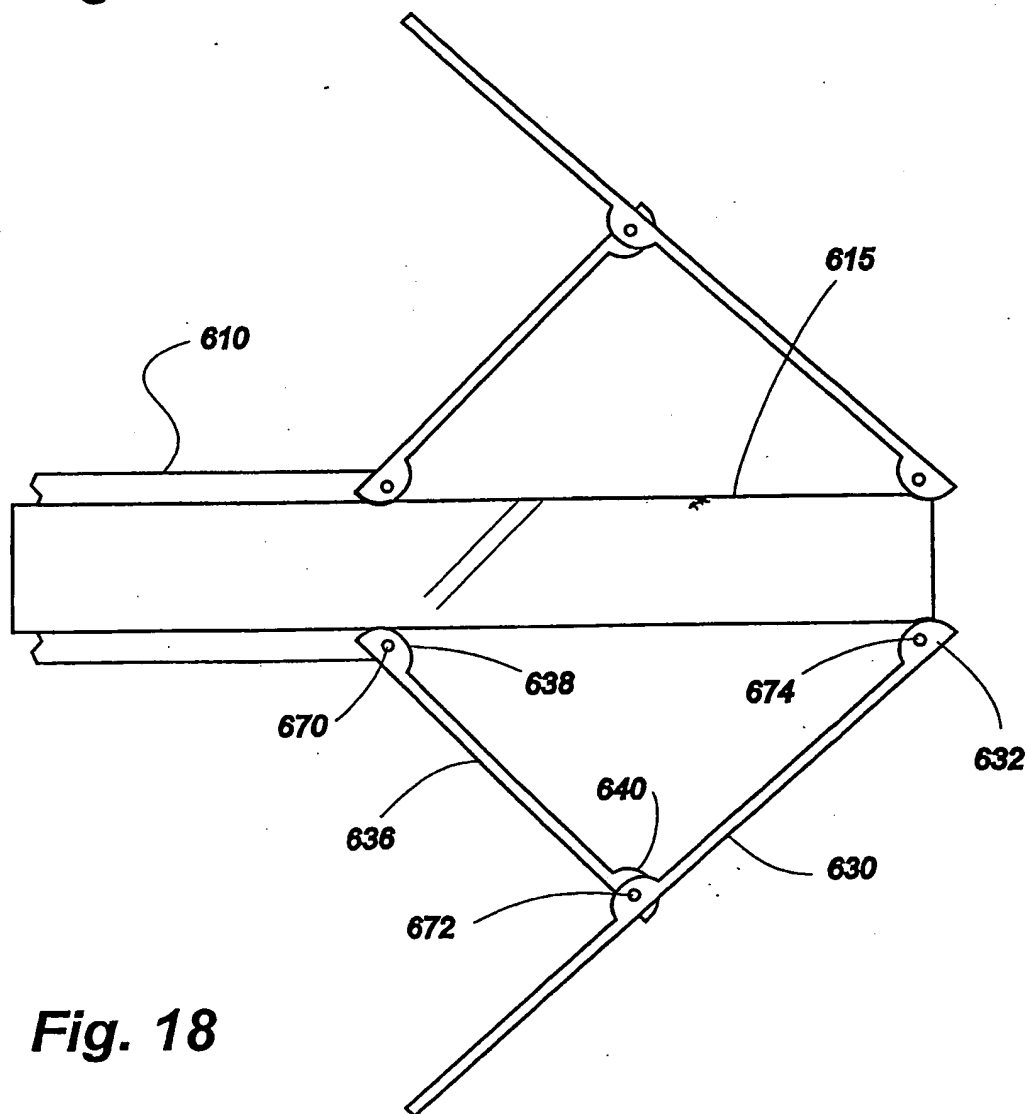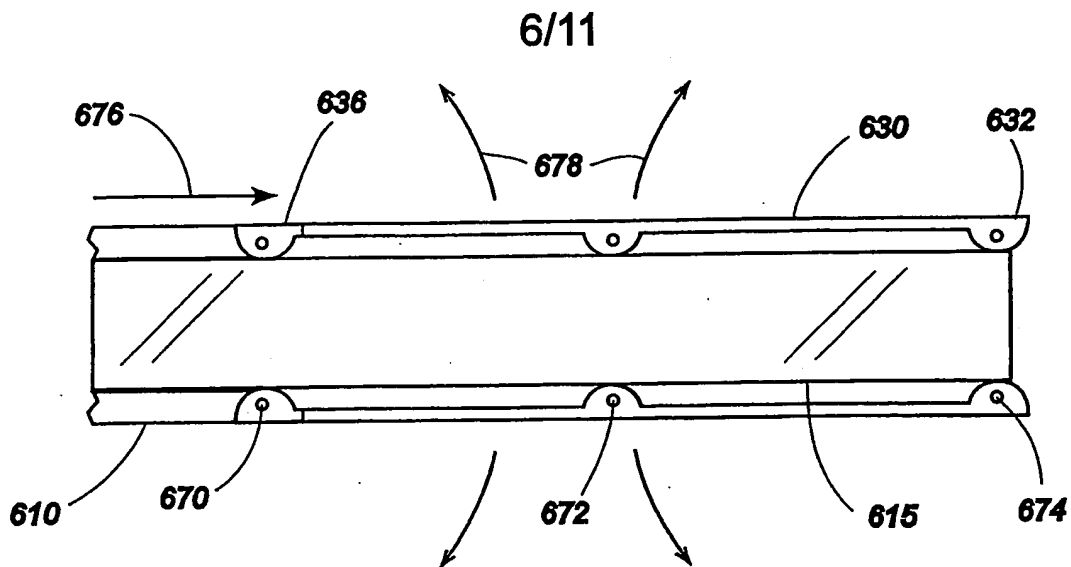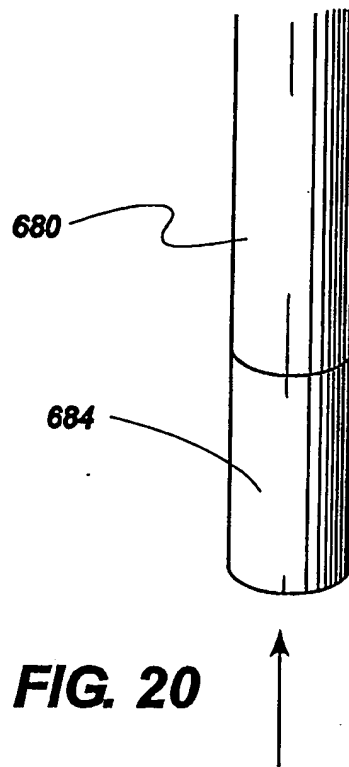

7/11

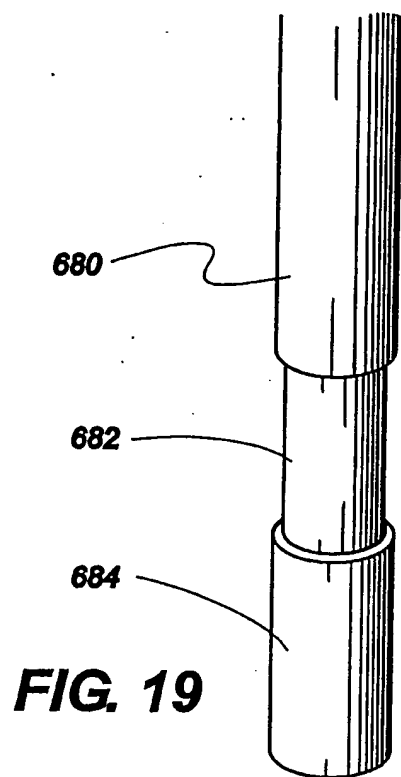

8/11

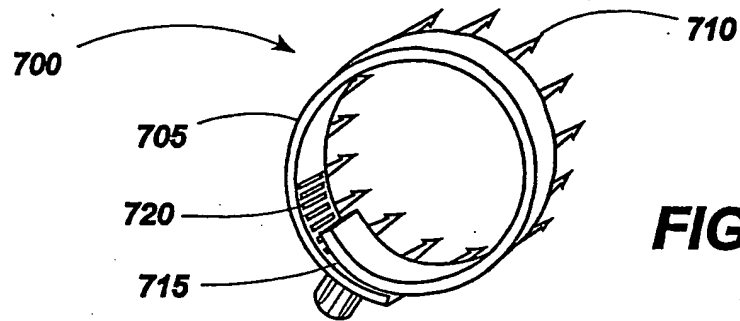


FIG. 21

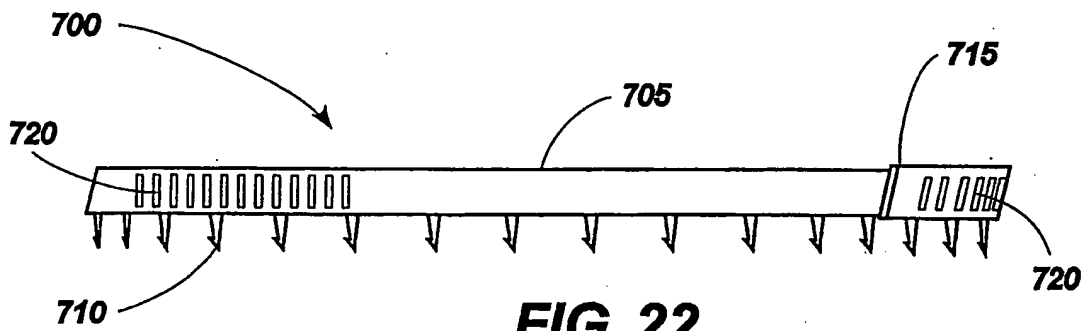


FIG. 22

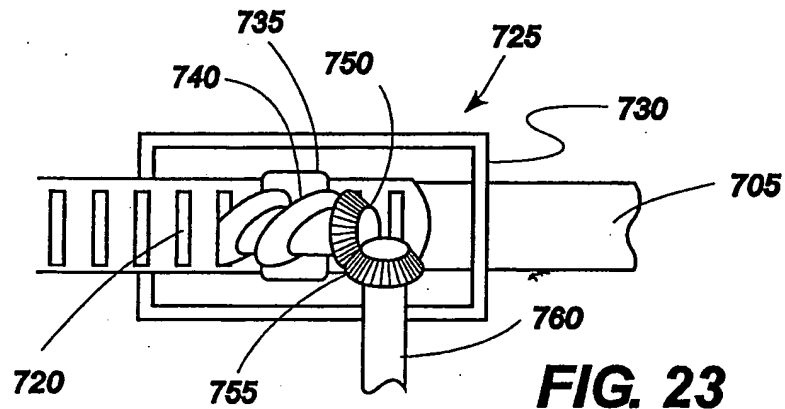


FIG. 23

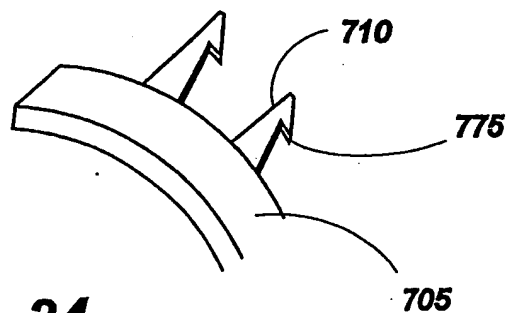


FIG. 24

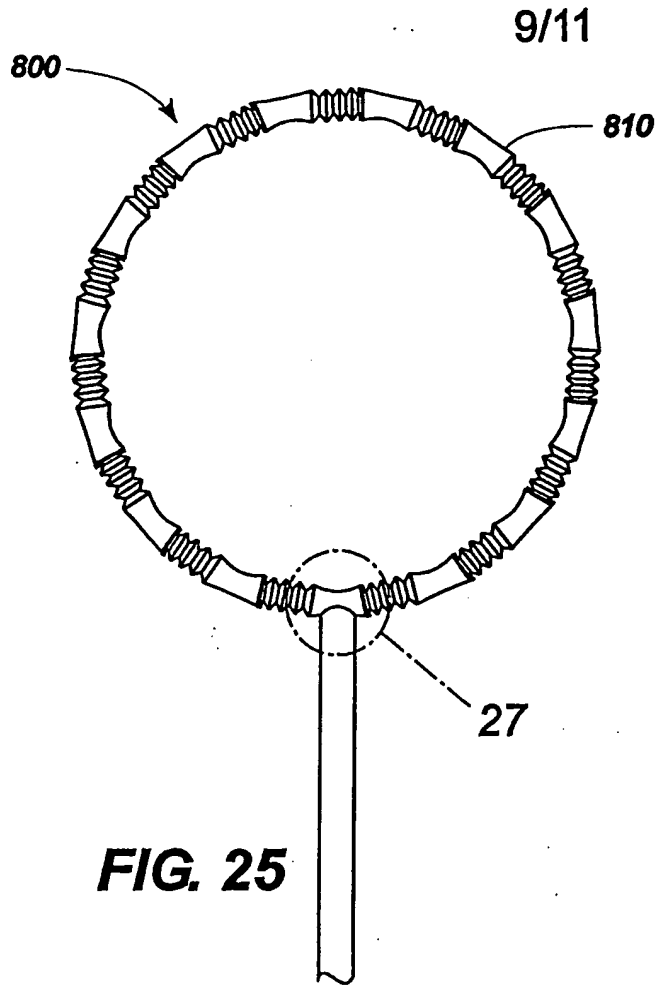


FIG. 25

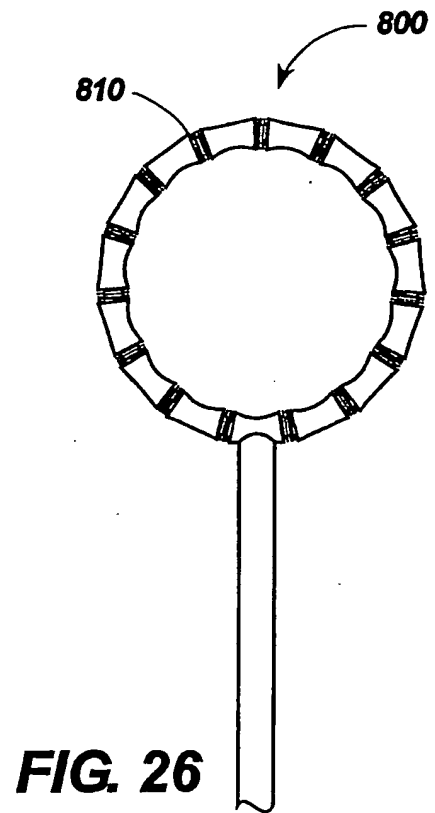


FIG. 26




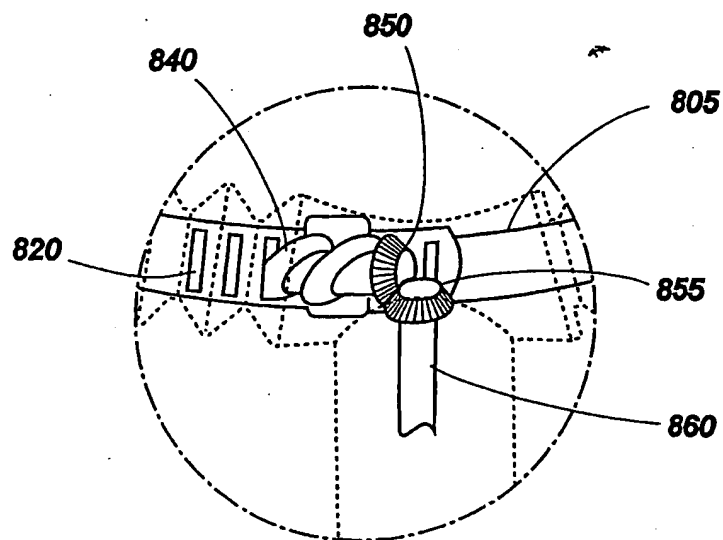


FIG. 27

10/11

**FIG. 28**

11/11

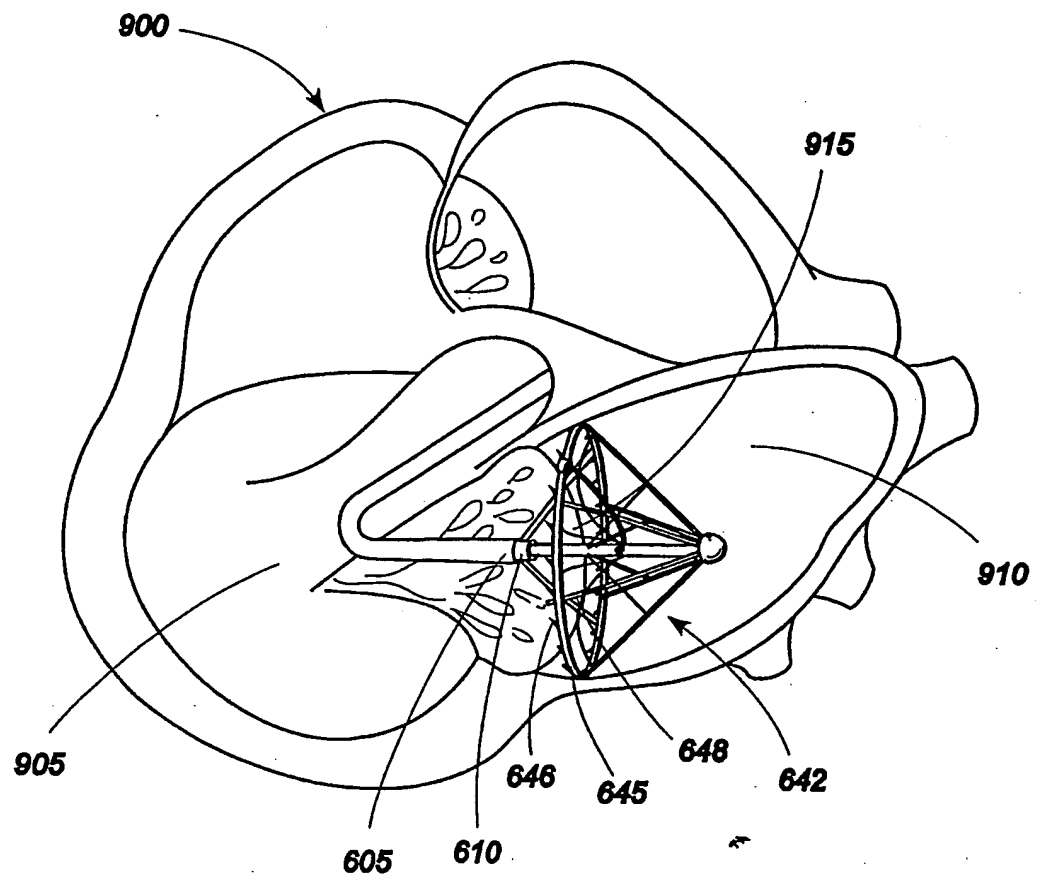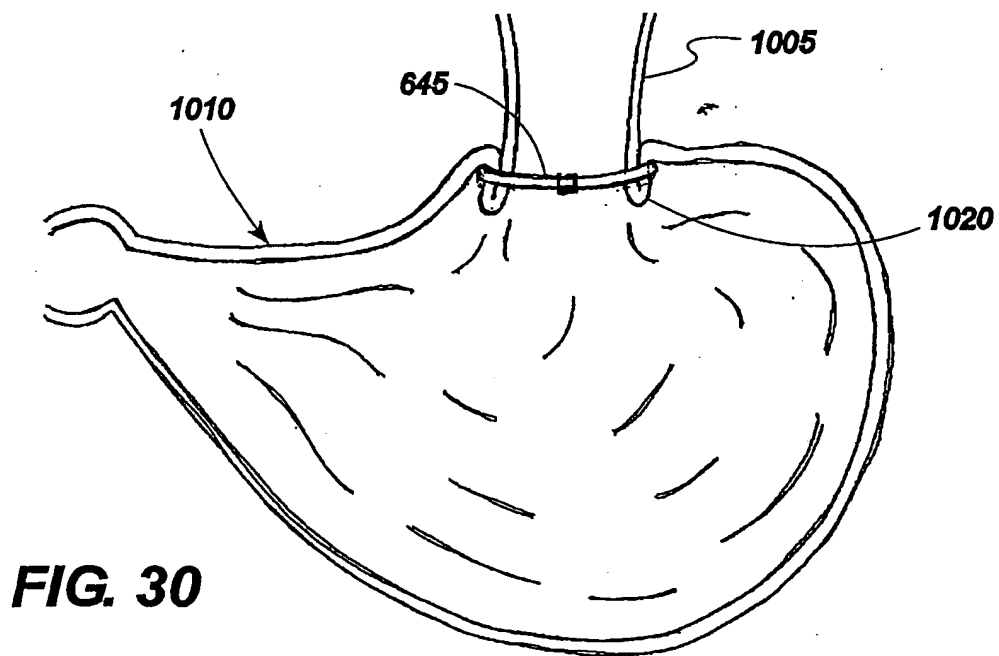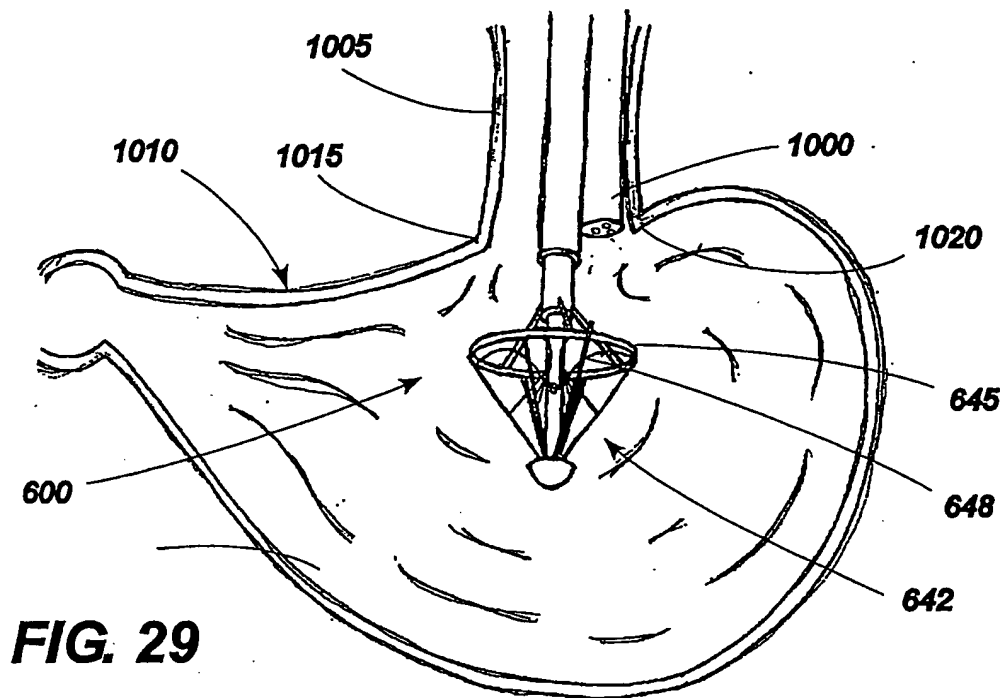

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
11 March 2004 (11.03.2004)

PCT

(10) International Publication Number
WO 2004/019816 A3

(51) International Patent Classification⁷: **A61F 2/24**

Richard, G. [US/US]; 1554 Yellow Heart Way, Hollywood, FL 30328 (US). LEE, Leonard, Y. [US/US]; 435 East 70th Street #12-L, New York, NY 10021 (US).

(21) International Application Number:
PCT/US2003/027278

(22) International Filing Date: 29 August 2003 (29.08.2003)

(74) Agents: ROBERTS, Larry, A. et al.; 1100 Peachtree Street, Suite 2800, Atlanta, GA 30309 (US).

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
60/406,841 29 August 2002 (29.08.2002) US
60/444,005 31 January 2003 (31.01.2003) US
60/447,383 14 February 2003 (14.02.2003) US
60/462,435 12 April 2003 (12.04.2003) US

(81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(71) Applicant (*for all designated States except US*): MD3 TECHNOLOGIES LLC [US/US]; Suite 3000, Five Concourse Parkway, Atlanta, GA 30328 (US).


(72) Inventors; and

(75) Inventors/Applicants (*for US only*): CARTLEDGE,

(84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

[Continued on next page]

(54) Title: IMPLANTABLE DEVICES FOR CONTROLLING THE INTERNAL CIRCUMFERENCE OF AN ANATOMIC ORIFICE OR LUMEN

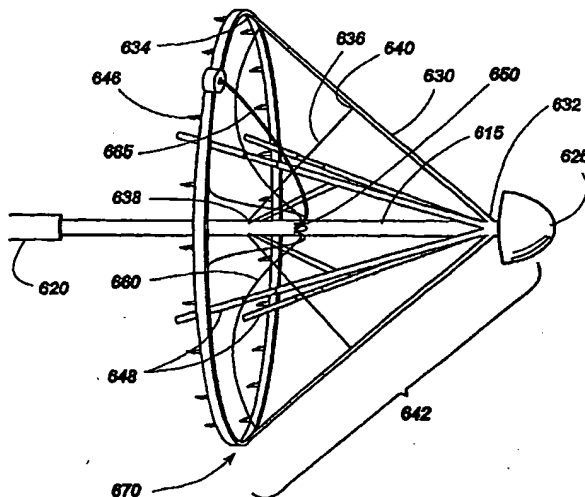

(57) Abstract: An implantable device (10, 100, 800) for controlling the circumference of internal anatomic passages corrects physiologic dysfunctions resulting from a structural lumen which is either too large or too small. Implants are disclosed which employ various means for adjusting and maintaining the size of an orifice to which they are attached. Systems permit the implants to be implanted using minimally invasive procedures and permit final adjustments to the circumference of the implants after the resumption of normal flow of anatomic fluids in situ. Methods are disclosed for using the implants to treat heart valve abnormalities, gastroesophageal abnormalities, anal incontinence, and the like.



Published:

- with international search report
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(88) Date of publication of the international search report:
26 August 2004

INTERNATIONAL SEARCH REPORT

International Application No.

PCT/US 03/27278

A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 A61F2/24

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61F

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X Y A	WO 99/04730 A (BAXTER INT) 4 February 1999 (1999-02-04) figures 15A,21-24 page 28, line 21 - line 22 -----	1,5,7,8, 12 2-4,6 9,10
X Y	US 6 419 696 B1 (SPENCE PAUL A ET AL) 16 July 2002 (2002-07-16) figures 5A,5B,12,13 column 2, line 10 - line 13 -----	1 2-4,6
X	US 6 406 493 B1 (QUIJANO RODOLFO C ET AL) 18 June 2002 (2002-06-18) figures 4,13 column 5, line 59 - line 60 column 7, line 12 - line 15 ----- -/-	1

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

3 March 2004

Date of mailing of the international search report

06. 07. 2004

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Franz, V

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 03/27278

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 6 368 348 B1 (GABBAY SHLOMO) 9 April 2002 (2002-04-09) figures 1A,1B	9,10
A	----- US 5 593 424 A (NORTHROP III WILLIAM F) 14 January 1997 (1997-01-14) the whole document -----	1-10,12

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US 03/27278

Box I Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:

2. ☐ Claims Nos.:
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:

3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box II Observations where unity of invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple inventions in this International application, as follows:

see additional sheet

1. ☐ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.

2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.

3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:

4. ☒ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

1-10, 12

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☐ No protest accompanied the payment of additional search fees.

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

This International Searching Authority found multiple (groups of) inventions in this international application, as follows:

1. claims: 1-10,12

Device for controlling internal circumference of anatomic orifice with grommets for fixation of the device at an orifice. The group of claims is directed towards the problem how to fix a device at an anatomic orifice.

2. claims: 1,11,13-23

Device for controlling internal circumference of anatomic orifice with adjustable diameter whereby the diameter can be chosen and is kept in place. The group of claims is directed towards the problem how to freely change the diameter of the device.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 03/27278

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 9904730	A	04-02-1999	AU 8497498 A CA 2297914 A1 EP 0996393 A1 WO 9904730 A1 US 6217610 B1 US 2001021874 A1	16-02-1999 04-02-1999 03-05-2000 04-02-1999 17-04-2001 13-09-2001
US 6419696	B1	16-07-2002	AU 6522501 A CA 2414022 A1 CN 1440261 T EP 1296618 A1 JP 2004502494 T WO 0203892 A1 US 2002173841 A1	21-01-2002 17-01-2002 03-09-2003 02-04-2003 29-01-2004 17-01-2002 21-11-2002
US 6406493	B1	18-06-2002	US 2003191528 A1	09-10-2003
US 6368348	B1	09-04-2002	CA 2409475 A1 EP 1294317 A1 JP 2003533275 T WO 0187191 A1	22-11-2001 26-03-2003 11-11-2003 22-11-2001
US 5593424	A	14-01-1997	AU 700530 B2 AU 3322495 A CA 2197069 A1 DE 69531105 D1 DE 69531105 T2 EP 0779793 A1 ES 2202369 T3 JP 10504481 T WO 9604852 A1 US 5709695 A ZA 9506672 A	07-01-1999 07-03-1996 22-02-1996 24-07-2003 06-05-2004 25-06-1997 01-04-2004 06-05-1998 22-02-1996 20-01-1998 04-07-1996

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

☐ BLACK BORDERS

☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES

☐ FADED TEXT OR DRAWING

☐ BLURRED OR ILLEGIBLE TEXT OR DRAWING

☐ SKEWED/SLANTED IMAGES

☒ COLOR OR BLACK AND WHITE PHOTOGRAPHS

☐ GRAY SCALE DOCUMENTS

☐ LINES OR MARKS ON ORIGINAL DOCUMENT

☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY

☐ OTHER: _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.